

**Department of Forensic Science**  
**Breath Alcohol Section**  
**Instrument Location History**  
**1/1/1990 To 6/12/2014**

---

**Instrument Serial Number:** 010537

**As of 12-Jun-14**

---

<b>Start Date</b>	<b>End Date</b>	<b>Agency Name</b>
12-Jun-14		Prince George County PD
30-May-14	12-Jun-14	DFS Central Lab
03-Apr-14	30-May-14	Bedford County SO
14-Mar-14	03-Apr-14	DFS Central Lab
03-May-10	14-Mar-14	Portsmouth PD
27-Apr-10	03-May-10	DFS Central Lab
12-Mar-09	27-Apr-10	Portsmouth PD
16-Jun-08	12-Mar-09	DFS Central Lab

TLN

# INTOX EC/IR II Quality Assurance Worksheet

Instrument Serial Number **010537** Worksheet Start Date **6/12/2014**

Location **Prince George PD**

Address **6600 Courthouse Rd Prince George VA 23875**

DFS Technician **Timmy Neece, Jr** License No. **25387**

Laboratory  On-Site

Site Specification: No detrimental environmental conditions exist.

Instrument Barometer (mm HG) **753** Reference Barometer (mm HG) **757**

Reference Barometer(RB)Serial # **009110** RB Calibration Due **5/28/2015**

### Measurement Assurance Check

<b>Standard (sea level)</b>	<b>PA Target</b>	<b>minimum</b>	<b>maximum</b>	<b>Sample 1</b>	<b>0.303</b>
0.300	0.297	0.288	0.305	<b>Sample 2</b>	<b>0.302</b>
<b>Precision</b>		<b>sample min</b>	<b>sample max</b>	<b>Sample 3</b>	<b>0.302</b>
0.001		0.302	0.303		


<b>Standard (sea level)</b>	<b>PA Target</b>	<b>minimum</b>	<b>maximum</b>	<b>Sample 1</b>	<b>0.101</b>
0.100	0.099	0.096	0.102	<b>Sample 2</b>	<b>0.101</b>
<b>Precision</b>		<b>sample min</b>	<b>sample max</b>	<b>Sample 3</b>	<b>0.100</b>
0.001		0.100	0.101		

Dry gas standard Lot No. (with tank no.) **AG227501-04**

- Replaced dry gas standard (+O-ring)
  - Installed at Location
  - Removed to DFS-Central
- Supplies  
Mouthpieces  
Certificates of Analysis  
Operator Worksheet  
Other:



Notes:

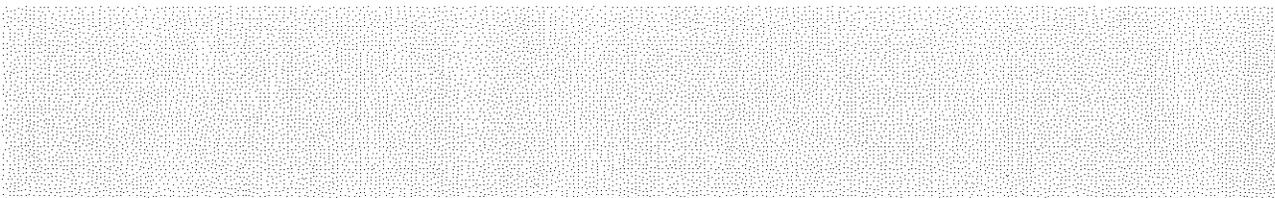

Instrument Serial Number

010537

Certification Date

Calibrated

Certified

Measurement Assurance Check

Instrument Test

Troubleshooting/Maintenance Worksheet Completed

(Successful completion denotes satisfactory condition of the item.)

<b>Standard (sea level)</b>	<b>PA Target</b>	<b>minimum</b>	<b>maximum</b>	<b>Sample 1</b>
0.250		0.000	0.000	<b>Sample 2</b>
<b>Precision</b>		<b>sample min</b>	<b>sample max</b>	<b>Sample 3</b>
0		0.000	0.000	

<b>Standard (sea level)</b>	<b>PA Target</b>	<b>minimum</b>	<b>maximum</b>	<b>Sample 1</b>
0.150		0.000	0.000	<b>Sample 2</b>
<b>Precision</b>		<b>sample min</b>	<b>sample max</b>	<b>Sample 3</b>
0		0.000	0.000	

<b>Standard (sea level)</b>	<b>PA Target</b>	<b>minimum</b>	<b>maximum</b>	<b>Sample 1</b>
0.080		-0.003	0.003	<b>Sample 2</b>
<b>Precision</b>		<b>sample min</b>	<b>sample max</b>	<b>Sample 3</b>
0		0.000	0.000	

<b>Standard (sea level)</b>	<b>PA Target</b>	<b>minimum</b>	<b>maximum</b>	<b>Sample 1</b>
0.020		-0.003	0.003	<b>Sample 2</b>
<b>Precision</b>		<b>sample min</b>	<b>sample max</b>	<b>Sample 3</b>
0		0.000	0.000	

All measurements are in g/210L

Estimation of Uncertainty of Measurement and traceability records are located within the Breath Alcohol Section

DFS Technician

*[Signature]*

Date

6/12/14

Issuing Analyst

*[Signature]*

Date

6/12/14

*[Signature]*

TLN

**Intox EC/IR-II: Accuracy Check**

*Department of Forensic Science*

Serial Number: 010537      Test Number: 1495

Test Date: 06/12/2014      Test Time: 10:50 EDT

Dry Gas Target: 0.297

Lot Number: AG334603-07      Exp Date: 12/12/2015

Tank Pressure: 272 psi      Barometric Pressure: 753 mmHg

System Check: *Passed*

Test	g/210L	Time
BLK	0.000	10:51
CHK	0.303	10:51
BLK	0.000	10:53
CHK	0.302	10:54
BLK	0.000	10:55
CHK	0.302	10:56

Test status: *Success*

Calibration CRC: 6B8E7224

TLN

**Intox EC/IR-II: Accuracy Check**

*Department of Forensic Science*

Serial Number: 010537      Test Number: 1496

Test Date: 06/12/2014      Test Time: 10:59 EDT

Dry Gas Target: 0.099

Lot Number: AG227501-04      Exp Date: 10/01/2014

Tank Pressure: 227 psi      Barometric Pressure: 753 mmHg

System Check: *Passed*

Test	g/210L	Time
BLK	0.000	11:00
CHK	0.101	11:00
BLK	0.000	11:02
CHK	0.101	11:03
BLK	0.000	11:04
CHK	0.100	11:05

Test Status: *Success*

Calibration CRC: 6B8E7224

TLN



COMMONWEALTH OF VIRGINIA  
DEPARTMENT OF FORENSIC SCIENCE

CERTIFICATE OF BLOOD ALCOHOL ANALYSIS  
AS DETERMINED BY A CHEMICAL TEST OF THE ACCUSED'S BREATH

NAME OF ACCUSED <b>INSTRUMENT, TEST,</b>	NAME OF COURT <b>DFS</b>
---	-----------------------------

BREATH ANALYSIS

SAMPLE EXAMINED AND TEST CONDUCTED BY <b>NEECE, JR., TIMMY, L</b>		AGENCY <b>DFS Central Lab</b>
DFS LICENSE NUMBER <b>25387</b>	LICENSE EXPIRES <b>10/01/2014</b>	DATE TEST CONDUCTED <b>06/12/2014</b>
TEST EQUIPMENT NUMBER <b>010537</b>		

RESULTS: TIME SAMPLE TAKEN 11:13 EDT

SAMPLE'S ALCOHOL CONTENT 0.00 GRAMS PER 210 LITERS OF BREATH

ATTEST:

I CERTIFY THAT THE ABOVE IS AN ACCURATE RECORD OF THE TEST CONDUCTED; THAT THE TEST WAS CONDUCTED WITH THE TYPE OF EQUIPMENT AND IN ACCORDANCE WITH THE METHODS APPROVED BY THE DEPARTMENT OF FORENSIC SCIENCE; THAT THE TEST WAS CONDUCTED IN ACCORDANCE WITH THE DEPARTMENT'S SPECIFICATIONS; THAT PRIOR TO ADMINISTRATION OF THE TEST THE ACCUSED WAS ADVISED OF HIS RIGHT TO OBSERVE THE PROCESS AND SEE THE BLOOD ALCOHOL READING ON THE EQUIPMENT USED TO PERFORM THE BREATH TEST, AND THAT I POSSESS A VALID LICENSE TO CONDUCT SUCH TEST, GIVEN UNDER MY HAND THIS \_\_\_\_\_ DAY OF \_\_\_\_\_, 20\_\_\_\_\_.

BREATH TEST OPERATOR

I HAVE RECEIVED A COPY OF THIS CERTIFICATE OF ANALYSIS \_\_\_\_\_ SUBJECT'S SIGNATURE

SUBJECT REFUSED TO SIGN FOR COPY OF CERTIFICATE OF ANALYSIS \_\_\_\_\_ OPERATOR'S SIGNATURE

FOR COURT



# IntoxNet MIS Report

Report Generated 12 Jun 2014 at 13:46

## Test Results

**Instrument Serial Number 010537**

**Test # 001497**      Subject Test

Test Location 1    Department of  
Test Date    12 Jun 2014

Test Location 2    Forensic Science  
Test Time    11:07  
Remote/Local    Local

Test Location 3  
System Check    Passed

Operator's Last Name    NEECE, JR.  
Agency    DFS Central Lab

Operator's First Name    TIMMY

Operator's Middle Initial    L

Card Serial Number    125387

License Number    25387

Effective Date    10/01/2012

Expiration Date    10/01/2014

Subject's Last Name    INSTRUMENT

Subject's First Name    TEST

Subject's Middle Initial

Subject's Date of Birth    00/00/0000

Subject's Sex    Male

Driver's License Number

Driver's License Expiration    00/00/0000

Driver's License State

Court Name    DFS

End Date    12 Jun 2014      End Time    11:15

Result Time    11:13

Result Date    12 Jun 2014      Result    0.00

Data Type    DIAG

Sample Value    Pass

Sample Time    11:08

Data Type    BLK

Sample Value    0.000

Sample Time    11:08

Data Type    CHK

Sample Value    0.100

Sample Time    11:09

Data Type    BLK

Sample Value    0.000

Sample Time    11:10

Data Type    SUBJ

Sample Value    0.000

Sample Time    11:11

Data Type    BLK

Sample Value    0.000

Sample Time    11:12

Data Type    SUBJ

Sample Value    0.000

Sample Time    11:13

Data Type    BLK

Sample Value    0.000

Sample Time    11:14

Standard Type    Dry Gas Std

Standard Value    0.099

Standard Lot Number    AG227501-04

Standard Expiration Date    10/01/2014

Tank Pressure    218

Barometric Pressure    752 mmHg

Blow Sample Number    1      Blow Duration    4.23 sec

Blow Volume    2068 cc      End-of-Blow Time    11:11

Blow Sample Number    2      Blow Duration    3.82 sec

Blow Volume    1958 cc      End-of-Blow Time    11:13

Tamper Evident Stamp    5843ec1b

Test Status Code    0

Test Status    Success