

TLN

**Department of Forensic Science  
Breath Alcohol Section  
Instrument Location History  
1/1/1990 To 8/18/2014**

---

**Instrument Serial Number: 010448**

**As of 18-Aug-14**

---

<b>Start Date</b>	<b>End Date</b>	<b>Agency Name</b>
15-Aug-14		DFS Central Lab
02-Apr-09	15-Aug-14	Newport News PD
23-Jun-08	02-Apr-09	DFS Central Lab

Department of Forensic Science  
Breath Alcohol Section  
Instrument Location History  
1/1/1990 To 8/18/2014

TLN

TLN 8/19/14

Instrument Serial Number: 010448 As of 18-Aug-14

Start Date	End Date	Agency Name
15-Aug-14		DFS Northern Regional Lab
02-Apr-09	15-Aug-14	Newport News PD
23-Jun-08	02-Apr-09	DFS Central Lab

Should be DFS Central Lab. TLN 8/19/14

# INTOX EC/IR II Quality Assurance Worksheet

Instrument Serial Number **010448** Worksheet Start Date **8/15/2014**  
 Location **Newport News PD North**  
 Address **368 Deshazor Dr Newport News VA 23608**  
 DFS Technician **Timmy Neece, Jr** License No. **25387**

Laboratory  On-Site

Site Specification: No detrimental environmental conditions exist.

Instrument Barometer (mm HG) **761** Reference Barometer (mm HG) **762**

Reference Barometer(RB)Serial # **009111** RB Calibration Due **5/19/2015**

### Measurement Assurance Check

<b>Standard (sea level)</b>	<b>PA Target</b>	<b>minimum</b>	<b>maximum</b>	<b>Sample 1</b>	0.305
0.300	0.300	0.291	0.309	<b>Sample 2</b>	0.305
<b>Precision</b>		<b>sample min</b>	<b>sample max</b>	<b>Sample 3</b>	0.304
0.001		0.304	0.305		

<b>Standard (sea level)</b>	<b>PA Target</b>	<b>minimum</b>	<b>maximum</b>	<b>Sample 1</b>	0.101
0.100	0.100	0.097	0.103	<b>Sample 2</b>	0.101
<b>Precision</b>		<b>sample min</b>	<b>sample max</b>	<b>Sample 3</b>	0.101
0		0.101	0.101		


Dry gas standard Lot No. (with tank no.) **AG400202-44**

Replaced dry gas standard (+O-ring)


Installed at Location

Removed to DFS-Central

Supplies  
Mouthpieces  
Certificates of Analysis  
Operator Worksheet  
Other:



Notes:

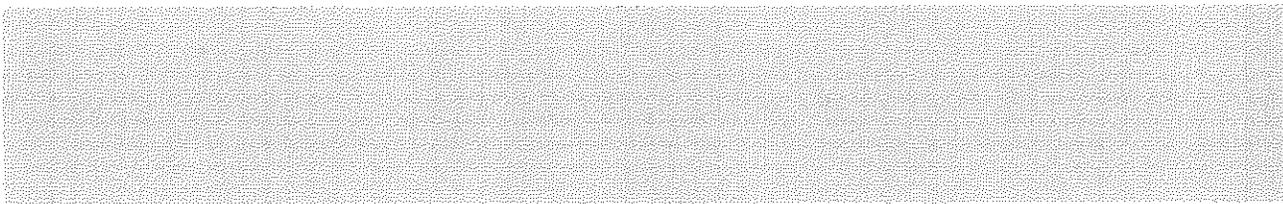

Instrument Serial Number

010448

Certification Date

Calibrated

Certified

Measurement Assurance Check

Instrument Test

Troubleshooting/Maintenance Worksheet Completed

(Successful completion denotes satisfactory condition of the item.)

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.250		0.000	0.000	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.150		0.000	0.000	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.080		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.020		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

All measurements are in g/210L

Estimation of Uncertainty of Measurement and traceability records are located within the Breath Alcohol Section

DFS Technician

Date

8/19/14

Issuing Analyst

Date

8/19/14

*mmb*

TLW



COMMONWEALTH OF VIRGINIA  
DEPARTMENT OF FORENSIC SCIENCE

CERTIFICATE OF BLOOD ALCOHOL ANALYSIS  
AS DETERMINED BY A CHEMICAL TEST OF THE ACCUSED'S BREATH

NAME OF ACCUSED <b>INSTRUMENT, TEST,</b>	NAME OF COURT <b>DFS</b>
---	-----------------------------

BREATH ANALYSIS

SAMPLE EXAMINED AND TEST CONDUCTED BY <b>NEECE, JR., TIMMY, L</b>		AGENCY <b>DFS Central Lab</b>
DFS LICENSE NUMBER <b>25387</b>	LICENSE EXPIRES <b>10/01/2014</b>	DATE TEST CONDUCTED <b>08/15/2014</b>
TEST EQUIPMENT NUMBER <b>010448</b>		

RESULTS: TIME SAMPLE TAKEN 10:34 EDT

SAMPLE'S ALCOHOL CONTENT 0.00 GRAMS PER 210 LITERS OF BREATH

ATTEST:

I CERTIFY THAT THE ABOVE IS AN ACCURATE RECORD OF THE TEST CONDUCTED; THAT THE TEST WAS CONDUCTED WITH THE TYPE OF EQUIPMENT AND IN ACCORDANCE WITH THE METHODS APPROVED BY THE DEPARTMENT OF FORENSIC SCIENCE; THAT THE TEST WAS CONDUCTED IN ACCORDANCE WITH THE DEPARTMENT'S SPECIFICATIONS; THAT PRIOR TO ADMINISTRATION OF THE TEST THE ACCUSED WAS ADVISED OF HIS RIGHT TO OBSERVE THE PROCESS AND SEE THE BLOOD ALCOHOL READING ON THE EQUIPMENT USED TO PERFORM THE BREATH TEST, AND THAT I POSSESS A VALID LICENSE TO CONDUCT SUCH TEST, GIVEN UNDER MY HAND THIS \_\_\_\_\_ DAY OF \_\_\_\_\_, 20 \_\_\_\_\_.

BREATH TEST OPERATOR
----------------------

I HAVE RECEIVED A COPY OF THIS CERTIFICATE OF ANALYSIS \_\_\_\_\_ SUBJECT'S SIGNATURE

SUBJECT REFUSED TO SIGN FOR COPY OF CERTIFICATE OF ANALYSIS \_\_\_\_\_ OPERATOR'S SIGNATURE

NMB  
TLN



# IntoxNet MIS Report

Report Generated 15 Aug 2014 at 10:59

## Test Results

**Instrument Serial Number 010448**

**Test # 001304**      Subject Test

Test Location 1    Department of  
Test Date    15 Aug 2014

Test Location 2    Forensic Science  
Test Time    10:28  
Remote/Local    Local

Test Location 3  
System Check    Passed

Operator's Last Name    NEECE,JR.  
Agency    DFS Central Lab

Operator's First Name    TIMMY

Operator's Middle Initial    L  
License Number    25387

Card Serial Number    125387

Effective Date    10/01/2012

Expiration Date    10/01/2014

Subject's Last Name    INSTRUMENT

Subject's First Name    TEST

Subject's Middle Initial

Subject's Date of Birth    00/00/0000

Subject's Sex    Male

Driver's License Number

Driver's License Expiration    00/00/0000

Driver's License State

Court Name    DFS

End Date    15 Aug 2014      End Time    10:35

Result Time    10:34

Result Date    15 Aug 2014      Result    0.00

Data Type    DIAG

Sample Value    Pass

Sample Time    10:28

Data Type    BLK

Sample Value    0.000

Sample Time    10:29

Data Type    CHK

Sample Value    0.101

Sample Time    10:30

Data Type    BLK

Sample Value    0.000

Sample Time    10:31

Data Type    SUBJ

Sample Value    0.000

Sample Time    10:32

Data Type    BLK

Sample Value    0.000

Sample Time    10:33

Data Type    SUBJ

Sample Value    0.000

Sample Time    10:34

Data Type    BLK

Sample Value    0.000

Sample Time    10:35

Standard Type    Dry Gas Std

Standard Value    0.100

Standard Lot Number    AG400202-44

Standard Expiration Date    01/02/2016

Tank Pressure    879

Barometric Pressure    761 mmHg

Blow Sample Number    1      Blow Duration    3.10 sec

Blow Volume    1713 cc      End-of-Blow Time    10:32

Blow Sample Number    2      Blow Duration    2.99 sec

Blow Volume    1833 cc      End-of-Blow Time    10:34

Tamper Evident Stamp    a7d32177

Test Status Code    0

Test Status    Success

TLN

**Intox EC/IR-II: Accuracy Check**

*Department of Forensic Science*

Serial Number: 010448      Test Number: 1305

Test Date: 08/15/2014      Test Time: 10:37 EDT

Dry Gas Target: 0.100

Lot Number: AG400202-44      Exp Date: 01/02/2016

Tank Pressure: 875 psi      Barometric Pressure: 761 mmHg

System Check: *Passed*

Test	g/210L	Time
BLK	0.000	10:37
CHK	0.101	10:38
BLK	0.000	10:40
CHK	0.101	10:40
BLK	0.000	10:42
CHK	0.101	10:43

Test Status: *Success*

Calibration CRC: 0845FB38

TLN

**Intox EC/IR-II: Accuracy Check**

*Department of Forensic Science*

Serial Number: 010448      Test Number: 1306

Test Date: 08/15/2014      Test Time: 10:46 EDT

Dry Gas Target: 0.300

Lot Number: AG334603-04      Exp Date: 12/12/2015

Tank Pressure: 139 psi      Barometric Pressure: 761 mmHg

System Check: *Passed*

Test	g/210L	Time
BLK	0.000	10:47
CHK	0.305	10:48
BLK	0.000	10:49
CHK	0.305	10:50
BLK	0.000	10:52
CHK	0.304	10:52

Test Status: *Success*

Calibration CRC: 0845FB38