

TLN

**Department of Forensic Science  
Breath Alcohol Section  
Instrument Location History  
1/1/1990 To 7/30/2014**

**Instrument Serial Number: 010472**

**As of 30-Jul-14**

<b>Start Date</b>	<b>End Date</b>	<b>Agency Name</b>
30-Jul-14		DFS Central Lab
21-Sep-12	30-Jul-14	Richmond PD
05-Sep-12	21-Sep-12	DFS Central Lab
14-Apr-09	05-Sep-12	Stafford County SO
19-May-08	14-Apr-09	DFS Central Lab

# INTOX EC/IR II Quality Assurance Worksheet

Instrument Serial Number **010472** Worksheet Start Date **7/30/2014**

Location **Richmond PD, 2nd Precinct**

Address **177 E. Belt Blvd. Richmond VA 23224**

DFS Technician **Timmy Neece, Jr** License No. **25387**

Laboratory  On-Site

Site Specification: No detrimental environmental conditions exist.

Instrument Barometer (mm HG) **759** Reference Barometer (mm HG) **759**

Reference Barometer(RB)Serial # **009111** RB Calibration Due **5/19/2015**

### Measurement Assurance Check


<b>Standard (sea level)</b>	<b>PA Target</b>	<b>minimum</b>	<b>maximum</b>	<b>Sample 1</b>	<b>0.305</b>
0.300	0.300	0.291	0.309	<b>Sample 2</b>	<b>0.305</b>
<b>Precision</b>		<b>sample min</b>	<b>sample max</b>	<b>Sample 3</b>	<b>0.304</b>
0.001		0.304	0.305		

<b>Standard (sea level)</b>	<b>PA Target</b>	<b>minimum</b>	<b>maximum</b>	<b>Sample 1</b>	<b>0.101</b>
0.100	0.100	0.097	0.103	<b>Sample 2</b>	<b>0.101</b>
<b>Precision</b>		<b>sample min</b>	<b>sample max</b>	<b>Sample 3</b>	<b>0.101</b>
0		0.101	0.101		


Dry gas standard Lot No. (with tank no.) **AG227501-03**

- Replaced dry gas standard (+O-ring)
- Installed at Location
- Removed to DFS-Central

Supplies  
Mouthpieces  
Certificates of Analysis  
Operator Worksheet  
Other:



Notes:

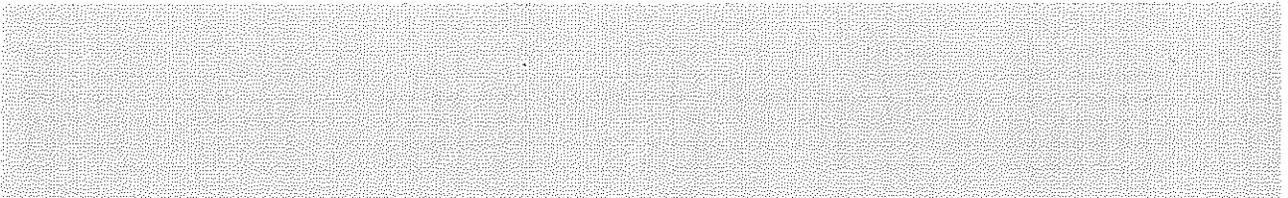

Instrument Serial Number

010472

Certification Date

Calibrated

Certified

Measurement Assurance Check

Instrument Test

Troubleshooting/Maintenance Worksheet Completed

(Successful completion denotes satisfactory condition of the item.)

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.250		0.000	0.000	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.150		0.000	0.000	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.080		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.020		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

All measurements are in g/210L

Estimation of Uncertainty of Measurement and traceability records are located within the Breath Alcohol Section

DFS Technician

Date

7/30/14

Issuing Analyst

Date

7/30/14

TLN



COMMONWEALTH OF VIRGINIA  
DEPARTMENT OF FORENSIC SCIENCE

CERTIFICATE OF BLOOD ALCOHOL ANALYSIS  
AS DETERMINED BY A CHEMICAL TEST OF THE ACCUSED'S BREATH

NAME OF ACCUSED  <b>INSTRUMENT, TEST,</b>	NAME OF COURT  <b>DFS</b>
---	---------------------------------

**BREATH ANALYSIS**

SAMPLE EXAMINED AND TEST CONDUCTED BY  <b>NEECE, JR., TIMMY, I.</b>		AGENCY  <b>DFS Central Lab</b>
DFS LICENSE NUMBER  <b>25387</b>	LICENSE EXPIRES  <b>10/01/2014</b>	DATE TEST CONDUCTED  <b>07/30/2014</b>
TEST EQUIPMENT NUMBER  <b>010472</b>		

RESULTS: TIME SAMPLE TAKEN 09:57 EDT

SAMPLE'S ALCOHOL CONTENT 0.00 GRAMS PER 210 LITERS OF BREATH

**ATTEST:**

I CERTIFY THAT THE ABOVE IS AN ACCURATE RECORD OF THE TEST CONDUCTED; THAT THE TEST WAS CONDUCTED WITH THE TYPE OF EQUIPMENT AND IN ACCORDANCE WITH THE METHODS APPROVED BY THE DEPARTMENT OF FORENSIC SCIENCE; THAT THE TEST WAS CONDUCTED IN ACCORDANCE WITH THE DEPARTMENT'S SPECIFICATIONS; THAT PRIOR TO ADMINISTRATION OF THE TEST THE ACCUSED WAS ADVISED OF HIS RIGHT TO OBSERVE THE PROCESS AND SEE THE BLOOD ALCOHOL READING ON THE EQUIPMENT USED TO PERFORM THE BREATH TEST, AND THAT I POSSESS A VALID LICENSE TO CONDUCT SUCH TEST, GIVEN UNDER MY HAND THIS \_\_\_\_\_ DAY OF \_\_\_\_\_, 20\_\_\_\_\_.

BREATH TEST OPERATOR
----------------------

I HAVE RECEIVED A COPY OF THIS CERTIFICATE OF ANALYSIS \_\_\_\_\_ SUBJECT'S SIGNATURE

SUBJECT REFUSED TO SIGN FOR COPY OF CERTIFICATE OF ANALYSIS \_\_\_\_\_ OPERATOR'S SIGNATURE

**FOR COURT**

TLV



# IntoxNet MIS Report

Report Generated 30 Jul 2014 at 11:31

## Test Results

**Instrument Serial Number 010472**

**Test # 002316**      **Subject Test**

**Test Location 1** Department of  
Test Date 30 Jul 2014

**Test Location 2** Forensic Science  
Test Time 09:51  
Remote/Local Local

**Test Location 3**  
System Check Passed

**Operator's Last Name** NEECE, JR.  
Agency DFS Central Lab

**Operator's First Name** TIMMY

**Operator's Middle Initial** L

**Card Serial Number** 125387

**License Number** 25387

**Effective Date** 10/01/2012

**Expiration Date** 10/01/2014

**Subject's Last Name** INSTRUMENT

**Subject's First Name** TEST

**Subject's Middle Initial**

**Subject's Date of Birth** 00/00/0000

**Subject's Sex** Male

**Driver's License Number**

**Driver's License Expiration** 00/00/0000

**Driver's License State**

**Court Name** DFS

**End Date** 30 Jul 2014      **End Time** 09:58

**Result Time** 09:57

**Result Date** 30 Jul 2014      **Result** 0.00

**Data Type** DIAG

**Sample Value** Pass

**Sample Time** 09:51

**Data Type** BLK

**Sample Value** 0.000

**Sample Time** 09:52

**Data Type** CHK

**Sample Value** 0.102

**Sample Time** 09:52

**Data Type** BLK

**Sample Value** 0.000

**Sample Time** 09:54

**Data Type** SUBJ

**Sample Value** 0.000

**Sample Time** 09:55

**Data Type** BLK

**Sample Value** 0.000

**Sample Time** 09:56

**Data Type** SUBJ

**Sample Value** 0.000

**Sample Time** 09:57

**Data Type** BLK

**Sample Value** 0.000

**Sample Time** 09:58

**Standard Type** Dry Gas Std

**Standard Value** 0.100

**Standard Lot Number** AG227501-03

**Standard Expiration Date** 10/01/2014

**Tank Pressure** 473

**Barometric Pressure** 759 mmHg

**Blow Sample Number** 1      **Blow Duration** 3.26 sec

**Blow Volume** 1915 cc      **End-of-Blow Time** 09:55

**Blow Sample Number** 2      **Blow Duration** 4.66 sec

**Blow Volume** 2356 cc      **End-of-Blow Time** 09:57

**Tamper Evident Stamp** db8c6419

**Test Status Code** 0

**Test Status** Success

TLW

**Intox EC/IR-II: Accuracy Check**

*Department of Forensic Science*

Serial Number: 010472      Test Number: 2317

Test Date: 07/30/2014      Test Time: 10:00 EDT

Dry Gas Target: 0.100

Lot Number: AG227501-03      Exp Date: 10/01/2014

Tank Pressure: 473 psi      Barometric Pressure: 759 mmHg

System Check: *Passed*

Test	g/210L	Time
BLK	0.000	10:00
CHK	0.101	10:01
BLK	0.000	10:03
CHK	0.101	10:03
BLK	0.000	10:05
CHK	0.101	10:05

Test Status: *Success*

Calibration CRC: 8CA0192A

TLW

**Intox EC/IR-11: Accuracy Check**

*Department of Forensic Science*

Serial Number: 010472      Test Number: 2318

Test Date: 07/30/2014      Test Time: 10:08 EDT

Dry Gas Target: 0.300

Lot Number: AG334603-04      Exp Date: 12/12/2015

Tank Pressure: 237 psi      Barometric Pressure: 759 mmHg

System Check: *Passed*

Test	g/210L	Time
BLK	0.000	10:09
CHK	0.305	10:10
BLK	0.000	10:11
CHK	0.305	10:12
BLK	0.000	10:14
CHK	0.304	10:14

Test Status: *Success*

Calibration CRC: 8CA0192A