

TLW

**Department of Forensic Science  
Breath Alcohol Section  
Instrument Location History  
1/1/1990 To 9/18/2014**

---

**Instrument Serial Number: 010545**

**As of 18-Sep-14**

---

<b>Start Date</b>	<b>End Date</b>	<b>Agency Name</b>
18-Sep-14		DFS Central Lab
15-Apr-14	18-Sep-14	Meherrin River Regional Jail
01-Apr-14	15-Apr-14	DFS Central Lab
21-Apr-09	01-Apr-14	Fairfax City PD
16-Jun-08	21-Apr-09	DFS Central Lab

TLN

# INTOX EC/IR II Quality Assurance Worksheet

Instrument Serial Number **010545** Worksheet Start Date **9/18/2014**  
 Location **Meherrin River <sup>Regional</sup> Satellite Jail - Mecklenburg Satellite**  
 Address **600 Prison Road Boydton, VA 23917**  
 DFS Technician **Timmy Neece, Jr** License No. **25387**

Laboratory  On-Site

Site Specification: No detrimental environmental conditions exist.

Instrument Barometer (mm HG) **752** Reference Barometer (mm HG) **754**  
 Reference Barometer(RB)Serial # **009111** RB Calibration Due **5/19/2015**

### Measurement Assurance Check


Standard (sea level)	PA Target	minimum	maximum	Sample 1	Sample 2	Sample 3
0.300	0.297	0.288	0.305	0.301	0.300	0.299
Precision		sample min	sample max			
0.002		0.299	0.301			

Standard (sea level)	PA Target	minimum	maximum	Sample 1	Sample 2	Sample 3
0.100	0.099	0.096	0.102	0.100	0.100	0.100
Precision		sample min	sample max			
0		0.100	0.100			


Dry gas standard Lot No. (with tank no.) **AG320502-02**

- Replaced dry gas standard (+O-ring)
- Installed at Location
- Removed to DFS-Central

- Supplies
- Mouthpieces
- Certificates of Analysis
- Operator Worksheet
- Other:



Notes:

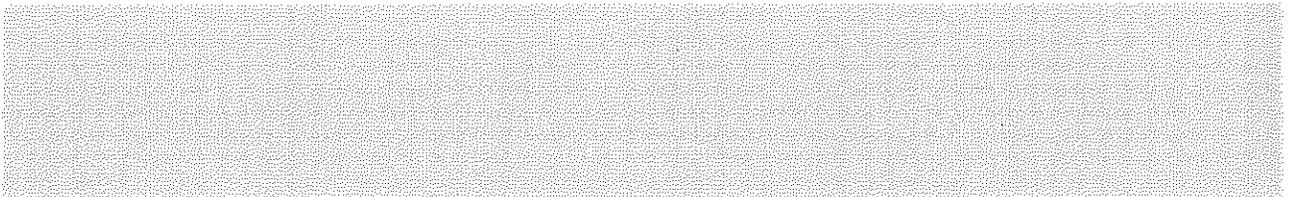

Instrument Serial Number

010545

Certification Date

Calibrated

Certified

Measurement Assurance Check

Instrument Test

Troubleshooting/Maintenance Worksheet Completed

(Successful completion denotes satisfactory condition of the item.)

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.250		0.000	0.000	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.150		0.000	0.000	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	


Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.080		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.020		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

All measurements are in g/210L

Estimation of Uncertainty of Measurement and traceability records are located within the Breath Alcohol Section

DFS Technician



Date

9/19/14

Issuing Analyst



Date

9/19/14

MSL

TLN



COMMONWEALTH OF VIRGINIA  
DEPARTMENT OF FORENSIC SCIENCE

CERTIFICATE OF BLOOD ALCOHOL ANALYSIS  
AS DETERMINED BY A CHEMICAL TEST OF THE ACCUSED'S BREATH

NAME OF ACCUSED <b>INSTRUMENT, TEST,</b>	NAME OF COURT <b>DFS</b>
---	-----------------------------

BREATH ANALYSIS

SAMPLE EXAMINED AND TEST CONDUCTED BY <b>NEECE, JR., TIMMY, L</b>		AGENCY <b>DFS Central Lab</b>
DFS LICENSE NUMBER <b>25387</b>	LICENSE EXPIRES <b>10/01/2014</b>	DATE TEST CONDUCTED <b>09/18/2014</b>
TEST EQUIPMENT NUMBER <b>010545</b>		

RESULTS: TIME SAMPLE TAKEN 10:02 EDT

SAMPLE'S ALCOHOL CONTENT 0.00 GRAMS PER 210 LITERS OF BREATH

ATTEST:

I CERTIFY THAT THE ABOVE IS AN ACCURATE RECORD OF THE TEST CONDUCTED; THAT THE TEST WAS CONDUCTED WITH THE TYPE OF EQUIPMENT AND IN ACCORDANCE WITH THE METHODS APPROVED BY THE DEPARTMENT OF FORENSIC SCIENCE; THAT THE TEST WAS CONDUCTED IN ACCORDANCE WITH THE DEPARTMENT'S SPECIFICATIONS; THAT PRIOR TO ADMINISTRATION OF THE TEST THE ACCUSED WAS ADVISED OF HIS RIGHT TO OBSERVE THE PROCESS AND SEE THE BLOOD ALCOHOL READING ON THE EQUIPMENT USED TO PERFORM THE BREATH TEST, AND THAT I POSSESS A VALID LICENSE TO CONDUCT SUCH TEST, GIVEN UNDER MY HAND THIS \_\_\_\_\_ DAY OF \_\_\_\_\_, 20\_\_\_\_\_.

BREATH TEST OPERATOR
----------------------

I HAVE RECEIVED A COPY OF THIS CERTIFICATE OF ANALYSIS \_\_\_\_\_ SUBJECT'S SIGNATURE

SUBJECT REFUSED TO SIGN FOR COPY OF CERTIFICATE OF ANALYSIS \_\_\_\_\_ OPERATOR'S SIGNATURE

FOR COURT



# IntoxNet MIS Report

Report Generated 18 Sep 2014 at 10:33

*mmB  
TLW*

## Test Results

**Instrument Serial Number 010545**

**Test # 000683**      Subject Test

Test Location 1    Department of  
Test Date    18 Sep 2014

Test Location 2    Forensic Science  
Test Time    09:56  
Remote/Local    Local

Test Location 3  
System Check    Passed

Operator's Last Name    NEECE, JR.  
Agency    DFS Central Lab

Operator's First Name    TIMMY

Operator's Middle Initial    L  
License Number    25387

Card Serial Number    125387  
Subject's Last Name    INSTRUMENT

Effective Date    10/01/2012      Expiration Date    10/01/2014

Subject's First Name    TEST

Subject's Middle Initial

Subject's Date of Birth    00/00/0000

Subject's Sex    Male

Driver's License Number

Driver's License Expiration    00/00/0000

Driver's License State

Court Name    DFS

End Date    18 Sep 2014      End Time    10:03      Result Time    10:02      Result Date    18 Sep 2014      Result    0.00

Data Type	DIAG	Sample Value	Pass	Sample Time	09:56
Data Type	BLK	Sample Value	0.000	Sample Time	09:57
Data Type	CHK	Sample Value	0.101	Sample Time	09:58
Data Type	BLK	Sample Value	0.000	Sample Time	09:59
Data Type	SUBJ	Sample Value	0.000	Sample Time	10:00
Data Type	BLK	Sample Value	0.000	Sample Time	10:01
Data Type	SUBJ	Sample Value	0.000	Sample Time	10:02
Data Type	BLK	Sample Value	0.000	Sample Time	10:03

Standard Type    Dry Gas Std

Standard Value    0.099

Standard Lot Number    AG320502-02

Standard Expiration Date    07/24/2015

Tank Pressure    634

Barometric Pressure    751 mmHg

Blow Sample Number    1      Blow Duration    2.74 sec

Blow Volume    1846 cc      End-of-Blow Time    10:00

Blow Sample Number    2      Blow Duration    2.48 sec

Blow Volume    1842 cc      End-of-Blow Time    10:02

Tamper Evident Stamp    5641bb1d

Test Status Code    0

Test Status    Success

TLW

**Intox EC/IR-II: Accuracy Check**

*Department of Forensic Science*

Serial Number: 010545      Test Number: 684

Test Date: 09/18/2014      Test Time: 10:05 EDT

Dry Gas Target: 0.099

Lot Number: AG320502-02      Exp Date: 07/24/2015

Tank Pressure: 629 psi      Barometric Pressure: 752 mmHg

System Check: *Passed*

Test	g/210L	Time
BLK	0.000	10:06
CHK	0.100	10:07
BLK	0.000	10:09
CHK	0.100	10:09
BLK	0.000	10:11
CHK	0.100	10:11

Test Status: *Success*

Calibration CRC: 12FC2C8E

**Intox EC/IR-II: Accuracy Check**

*Department of Forensic Science*

Serial Number: 010545      Test Number: 685

Test Date: 09/18/2014      Test Time: 10:14 EDT

Dry Gas Target: 0.297

Lot Number: AG421201-04      Exp Date: 07/31/2016

Tank Pressure: 433 psi      Barometric Pressure: 752 mmHg

System Check: *Passed*

Test	g/210L	Time
BLK	0.000	10:15
CHK	0.301	10:16
BLK	0.000	10:18
CHK	0.300	10:19
BLK	0.000	10:20
CHK	0.299	10:21

Test Status: *Success*

Calibration CRC: 12FC2C8E