

FLN

**Department of Forensic Science
Breath Alcohol Section
Instrument Location History
1/1/1990 To 9/18/2014**

Instrument Serial Number: 010550

As of 18-Sep-14

Start Date	End Date	Agency Name
18-Sep-14		Chase City PD
04-Sep-14	18-Sep-14	DFS Central Lab
18-Mar-14	04-Sep-14	Chesapeake Bay Bridge
11-Mar-14	18-Mar-14	DFS Central Lab
13-Nov-08	11-Mar-14	Charlotte County SO
16-Jun-08	13-Nov-08	DFS Central Lab

TLW

INTOX EC/IR II Quality Assurance Worksheet

Instrument Serial Number **010550** Worksheet Start Date **9/18/2014**

Location **Chase City PD**

Address **219 E 2nd St Chase City VA 23924**

DFS Technician **Timmy Neece, Jr** License No. **25387**

Laboratory On-Site

Site Specification: No detrimental environmental conditions exist.

Instrument Barometer (mm HG) **747** Reference Barometer (mm HG) **747**

Reference Barometer(RB)Serial # **009111** RB Calibration Due **5/19/2015**

Measurement Assurance Check

Standard (sea level)	PA Target	minimum	maximum	Sample 1	0.300
0.300	0.295	0.286	0.303	Sample 2	0.298
Precision		sample min	sample max	Sample 3	0.298
0.002		0.298	0.300		

Standard (sea level)	PA Target	minimum	maximum	Sample 1	0.099
0.100	0.098	0.095	0.101	Sample 2	0.098
Precision		sample min	sample max	Sample 3	0.098
0.001		0.098	0.099		


Dry gas standard Lot No. (with tank no.) **AG316301-22**

- Replaced dry gas standard (+O-ring)
- Installed at Location
- Removed to DFS-Central

Supplies
Mouthpieces
Certificates of Analysis
Operator Worksheet
Other:



Notes:

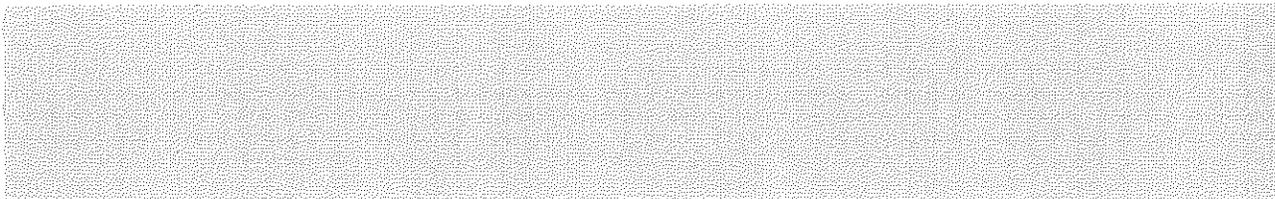

Instrument Serial Number

010550

Certification Date

Calibrated

Certified

Measurement Assurance Check

Instrument Test

Troubleshooting/Maintenance Worksheet Completed

(Successful completion denotes satisfactory condition of the item.)

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.250		0.000	0.000	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.150		0.000	0.000	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.080		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.020		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

All measurements are in g/210L

Estimation of Uncertainty of Measurement and traceability records are located within the Breath Alcohol Section

DFS Technician

Date

9/19/14

Issuing Analyst

Date

9/19/14

msk

TLN

Intox EC/IR-II: Accuracy Check

Department of Forensic Science

Serial Number: 010550 Test Number: 646

Test Date: 09/18/2014 Test Time: 12:17 EDT

Dry Gas Target: 0.295

Lot Number: AG421201-04 Exp Date: 07/31/2016

Tank Pressure: 428 psi Barometric Pressure: 747 mmHg

System Check: *Passed*

Test	g/210L	Time
BLK	0.000	12:18
CHK	0.300	12:18
BLK	0.000	12:20
CHK	0.298	12:21
BLK	0.000	12:22
CHK	0.298	12:23

Test Status: *Success*

Calibration CRC: 95BC3BE2

TLN

Intox EC/IR-II: Accuracy Check

Department of Forensic Science

Serial Number: 010550 Test Number: 647

Test Date: 09/18/2014 Test Time: 12:28 EDT

Dry Gas Target: 0.098

Lot Number: AG316301-22 Exp Date: 06/12/2015

Tank Pressure: 223 psi Barometric Pressure: 747 mmHg

System Check: *Passed*

Test	g/210L	Time
BLK	0.000	12:28
CHK	0.099	12:29
BLK	0.000	12:31
CHK	0.098	12:32
BLK	0.000	12:33
CHK	0.098	12:34

Test Status: *Success*

Calibration CRC: 95BC3BE2

TW



COMMONWEALTH OF VIRGINIA
DEPARTMENT OF FORENSIC SCIENCE

CERTIFICATE OF BLOOD ALCOHOL ANALYSIS
AS DETERMINED BY A CHEMICAL TEST OF THE ACCUSED'S BREATH

NAME OF ACCUSED INSTRUMENT, TEST,	NAME OF COURT DFS
---	-----------------------------

BREATH ANALYSIS

SAMPLE EXAMINED AND TEST CONDUCTED BY NEECE, JR., TIMMY, L		AGENCY DFS Central Lab
DFS LICENSE NUMBER 25387	LICENSE EXPIRES 10/01/2014	DATE TEST CONDUCTED 09/18/2014
TEST EQUIPMENT NUMBER 010550		

RESULTS: TIME SAMPLE TAKEN 12:42 EDT

SAMPLE'S ALCOHOL CONTENT 0.00 GRAMS PER 210 LITERS OF BREATH

ATTEST:

I CERTIFY THAT THE ABOVE IS AN ACCURATE RECORD OF THE TEST CONDUCTED; THAT THE TEST WAS CONDUCTED WITH THE TYPE OF EQUIPMENT AND IN ACCORDANCE WITH THE METHODS APPROVED BY THE DEPARTMENT OF FORENSIC SCIENCE; THAT THE TEST WAS CONDUCTED IN ACCORDANCE WITH THE DEPARTMENT'S SPECIFICATIONS; THAT PRIOR TO ADMINISTRATION OF THE TEST THE ACCUSED WAS ADVISED OF HIS RIGHT TO OBSERVE THE PROCESS AND SEE THE BLOOD ALCOHOL READING ON THE EQUIPMENT USED TO PERFORM THE BREATH TEST, AND THAT I POSSESS A VALID LICENSE TO CONDUCT SUCH TEST, GIVEN UNDER MY HAND THIS _____ DAY OF _____, 20_____.

BREATH TEST OPERATOR

I HAVE RECEIVED A COPY OF THIS CERTIFICATE OF ANALYSIS _____ SUBJECT'S SIGNATURE

SUBJECT REFUSED TO SIGN FOR COPY OF CERTIFICATE OF ANALYSIS _____ OPERATOR'S SIGNATURE

TLN



IntoxNet MIS Report

Report Generated 18 Sep 2014 at 15:34

Test Results

Instrument Serial Number 010550

Test # 000648 **Subject Test**

Test Location 1 Department of Test Date 18 Sep 2014	Test Location 2 Forensic Science Test Time 12:36 Remote/Local Local	Test Location 3 System Check Passed
Operator's Last Name NEECE, JR. Agency DFS Central Lab	Operator's First Name TIMMY	Operator's Middle Initial L
Card Serial Number 125387	Effective Date 10/01/2012	License Number 25387
Subject's Last Name INSTRUMENT	Subject's First Name TEST	Expiration Date 10/01/2014
Subject's Middle Initial	Subject's Date of Birth 00/00/0000	Subject's Sex Male
Driver's License Number		Driver's License Expiration 00/00/0000
Driver's License State	Court Name DFS	
End Date 18 Sep 2014 End Time 12:44	Result Time 12:42	Result Date 18 Sep 2014 Result 0.00
Data Type DIAG	Sample Value Pass	Sample Time 12:37
Data Type BLK	Sample Value 0.000	Sample Time 12:37
Data Type CHK	Sample Value 0.098	Sample Time 12:38
Data Type BLK	Sample Value 0.000	Sample Time 12:39
Data Type SUBJ	Sample Value 0.000	Sample Time 12:40
Data Type BLK	Sample Value 0.000	Sample Time 12:41
Data Type SUBJ	Sample Value 0.000	Sample Time 12:42
Data Type BLK	Sample Value 0.000	Sample Time 12:43
Standard Type Dry Gas Std		Standard Value 0.098
Standard Lot Number AG316301-22		Standard Expiration Date 06/12/2015
Tank Pressure 213		Barometric Pressure 746 mmHg
Blow Sample Number 1 Blow Duration 3.26 sec	Blow Volume 1830 cc	End-of-Blow Time 12:40
Blow Sample Number 2 Blow Duration 3.20 sec	Blow Volume 2007 cc	End-of-Blow Time 12:42
Tamper Evident Stamp d13cf301		Test Status Code 0
Test Status Success		