

TLV

Department of Forensic Science
Breath Alcohol Section
Instrument Location History
1/1/1990 To 10/21/2014

Instrument Serial Number: 010596

As of 21-Oct-14

Start Date	End Date	Agency Name
21-Oct-14		DFS Central Lab
23-May-14	21-Oct-14	West Point PD
21-May-14	23-May-14	DFS Central Lab
13-Nov-08	21-May-14	Bath County SO
15-Aug-08	13-Nov-08	DFS Central Lab

TLW

INTOX EC/IR II Quality Assurance Worksheet

Instrument Serial Number **010596** Worksheet Start Date **10/21/2014**
 Location **West Point PD**
 Address **433 12th St West Point VA 23181**
 DFS Technician **Timmy Neece, Jr** License No. **25387**

Laboratory On-Site

Site Specification: No detrimental environmental conditions exist.

Instrument Barometer (mm HG) **756** Reference Barometer (mm HG) **760**
 Reference Barometer(RB)Serial # **009111** RB Calibration Due **5/19/2015**

Measurement Assurance Check

Standard (sea level)	PA Target	minimum	maximum	Sample 1	0.303
0.300	0.298	0.289	0.306	Sample 2	0.303
Precision		sample min	sample max	Sample 3	0.302
0.001		0.302	0.303		

Standard (sea level)	PA Target	minimum	maximum	Sample 1	0.102
0.100	0.100	0.097	0.103	Sample 2	0.102
Precision		sample min	sample max	Sample 3	0.101
0.001		0.101	0.102		


Dry gas standard Lot No. (with tank no.) **AG320502-10**

- Replaced dry gas standard (+O-ring)
- Installed at Location
- Removed to DFS-Central

Supplies
 Mouthpieces
 Certificates of Analysis
 Operator Worksheet
 Other:



Notes:

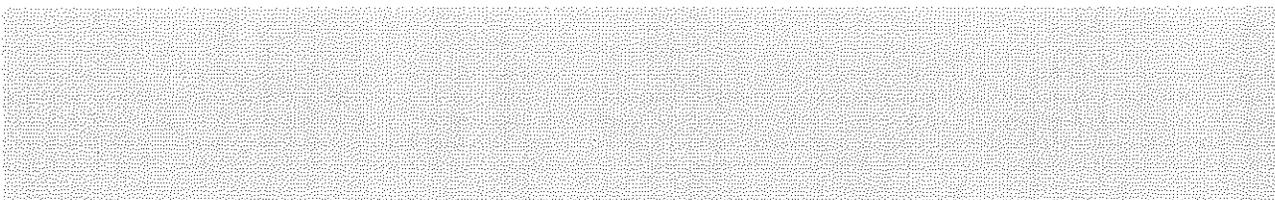

Instrument Serial Number

010596

Certification Date

Calibrated

Certified

Measurement Assurance Check

Instrument Test

Troubleshooting/Maintenance Worksheet Completed

(Successful completion denotes satisfactory condition of the item.)

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.250		0.000	0.000	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.150		0.000	0.000	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.080		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.020		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

All measurements are in g/210L

Estimation of Uncertainty of Measurement and traceability records are located within the Breath Alcohol Section

DFS Technician

[Signature]

Date

10/21/14

Issuing Analyst

[Signature]

Date

10/21/14

MB

TLN



COMMONWEALTH OF VIRGINIA
DEPARTMENT OF FORENSIC SCIENCE

CERTIFICATE OF BLOOD ALCOHOL ANALYSIS
AS DETERMINED BY A CHEMICAL TEST OF THE ACCUSED'S BREATH

NAME OF ACCUSED INSTRUMENT, TEST,	NAME OF COURT DFS
---	-----------------------------

BREATH ANALYSIS

SAMPLE EXAMINED AND TEST CONDUCTED BY NEECE, JR., TIMMY, L		AGENCY DFS Central Lab
DFS LICENSE NUMBER 25387	LICENSE EXPIRES 10/01/2016	DATE TEST CONDUCTED 10/21/2014
TEST EQUIPMENT NUMBER 010596		

RESULTS: TIME SAMPLE TAKEN 08:58 EDT

SAMPLE'S ALCOHOL CONTENT 0.00 GRAMS PER 210 LITERS OF BREATH

ATTEST:

I CERTIFY THAT THE ABOVE IS AN ACCURATE RECORD OF THE TEST CONDUCTED; THAT THE TEST WAS CONDUCTED WITH THE TYPE OF EQUIPMENT AND IN ACCORDANCE WITH THE METHODS APPROVED BY THE DEPARTMENT OF FORENSIC SCIENCE; THAT THE TEST WAS CONDUCTED IN ACCORDANCE WITH THE DEPARTMENT'S SPECIFICATIONS; THAT PRIOR TO ADMINISTRATION OF THE TEST THE ACCUSED WAS ADVISED OF HIS RIGHT TO OBSERVE THE PROCESS AND SEE THE BLOOD ALCOHOL READING ON THE EQUIPMENT USED TO PERFORM THE BREATH TEST, AND THAT I POSSESS A VALID LICENSE TO CONDUCT SUCH TEST, GIVEN UNDER MY HAND THIS _____ DAY OF _____, 20_____.

BREATH TEST OPERATOR

I HAVE RECEIVED A COPY OF THIS CERTIFICATE OF ANALYSIS _____ SUBJECT'S SIGNATURE

SUBJECT REFUSED TO SIGN FOR COPY OF CERTIFICATE OF ANALYSIS _____ OPERATOR'S SIGNATURE

TW



IntoxNet MIS Report

Report Generated 21 Oct 2014 at 13:39

Test Results

Instrument Serial Number 010596

Test # 000310	Subject Test	Test Location 2 Forensic Science	Test Location 3
Test Location 1 Department of		Test Time 08:52	System Check Passed
Test Date 21 Oct 2014		Remote/Local Local	
Operator's Last Name NEECE, JR.		Operator's First Name TIMMY	Operator's Middle Initial L
Agency DFS Central Lab		License Number 25387	
Card Serial Number 125387		Effective Date 10/01/2014	Expiration Date 10/01/2016
Subject's Last Name INSTRUMENT		Subject's First Name TEST	
Subject's Middle Initial		Subject's Date of Birth 00/00/0000	Subject's Sex Male
Driver's License Number		Driver's License Expiration 00/00/0000	
Driver's License State		Court Name DFS	
End Date 21 Oct 2014	End Time 08:59	Result Time 08:58	Result Date 21 Oct 2014
Data Type DIAG		Sample Value Pass	Sample Time 08:52
Data Type BLK		Sample Value 0.000	Sample Time 08:53
Data Type CHK		Sample Value 0.102	Sample Time 08:53
Data Type BLK		Sample Value 0.000	Sample Time 08:55
Data Type SUBJ		Sample Value 0.000	Sample Time 08:56
Data Type BLK		Sample Value 0.000	Sample Time 08:57
Data Type SUBJ		Sample Value 0.000	Sample Time 08:58
Data Type BLK		Sample Value 0.000	Sample Time 08:59
Standard Type Dry Gas Std		Standard Value 0.100	
Standard Lot Number AG320502-10		Standard Expiration Date 07/24/2015	
Tank Pressure 747		Barometric Pressure 757 mmHg	
Blow Sample Number 1	Blow Duration 3.05 sec	Blow Volume 1904 cc	End-of-Blow Time 08:56
Blow Sample Number 2	Blow Duration 3.19 sec	Blow Volume 1807 cc	End-of-Blow Time 08:58
Tamper Evident Stamp 82f82137		Test Status Code 0	
Test Status Success			

TLN

Intox EC/IR-II: Accuracy Check

Department of Forensic Science

Serial Number: 010596 Test Number: 311

Test Date: 10/21/2014 Test Time: 09:01 EDT

Dry Gas Target: 0.100

Lot Number: AG320502-10 Exp Date: 07/24/2015

Tank Pressure: 742 psi Barometric Pressure: 756 mmHg

System Check: *Passed*

Test	g/210L	Time
BLK	0.000	09:02
CHK	0.102	09:03
BLK	0.000	09:04
CHK	0.102	09:05
BLK	0.000	09:06
CHK	0.101	09:07

Test Status: *Success*

Calibration CRC: 2935AE90

TLN

Intox EC/IR-II: Accuracy Check

Department of Forensic Science

Serial Number: 010596 Test Number: 312

Test Date: 10/21/2014 Test Time: 09:10 EDT

Dry Gas Target: 0.298

Lot Number: AG421201-03 Exp Date: 07/31/2016

Tank Pressure: 438 psi Barometric Pressure: 756 mmHg

System Check: *Passed*

Test	g/210L	Time
BLK	0.000	09:10
CHK	0.303	09:11
BLK	0.000	09:13
CHK	0.303	09:14
BLK	0.000	09:15
CHK	0.302	09:16

Test Status: *Success*

Calibration CRC: 2935AE90