

T/W

**Department of Forensic Science
Breath Alcohol Section
Instrument Location History
1/1/1990 To 11/19/2014**

Instrument Serial Number: 010537

As of 19-Nov-14

Start Date	End Date	Agency Name
19-Nov-14		DFS Central Lab
12-Jun-14	19-Nov-14	Prince George County PD
30-May-14	12-Jun-14	DFS Central Lab
03-Apr-14	30-May-14	Bedford County SO
14-Mar-14	03-Apr-14	DFS Central Lab
03-May-10	14-Mar-14	Portsmouth PD
27-Apr-10	03-May-10	DFS Central Lab
12-Mar-09	27-Apr-10	Portsmouth PD
16-Jun-08	12-Mar-09	DFS Central Lab

TLN

INTOX EC/IR II Quality Assurance Worksheet

Instrument Serial Number **010537** Worksheet Start Date **11/19/2014**
 Location **Prince George PD**
 Address **6600 Courthouse Rd Prince George VA 23875**
 DFS Technician **Timmy Neece, Jr.** License No. **25387**

Laboratory On-Site

Site Specification: No detrimental environmental conditions exist.

Instrument Barometer (mm HG) **765** Reference Barometer (mm HG) **769**

Reference Barometer(RB)Serial # **009111** RB Calibration Due **5/19/2015**

Measurement Assurance Check


Standard (sea level)	PA Target	minimum	maximum	Sample 1	Sample 2	Sample 3
0.300	0.302	0.292	0.311	0.308	0.308	0.307
Precision		sample min	sample max			
0.001		0.307	0.308			

Standard (sea level)	PA Target	minimum	maximum	Sample 1	Sample 2	Sample 3
0.100	0.101	0.097	0.104	0.102	0.102	0.102
Precision		sample min	sample max			
0		0.102	0.102			


Dry gas standard Lot No. (with tank no.) **AG320502-04**

- Replaced dry gas standard (+O-ring)
- Installed at Location
- Removed to DFS-Central

Supplies
Mouthpieces
Certificates of Analysis
Operator Worksheet
Other:



Notes:

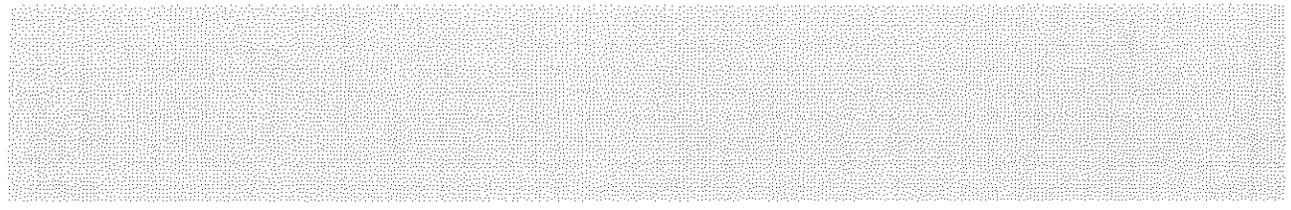

Instrument Serial Number

010537

Certification Date

Calibrated

Certified

Measurement Assurance Check

Instrument Test

Troubleshooting/Maintenance Worksheet Completed

(Successful completion denotes satisfactory condition of the item.)

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.250		0.000	0.000	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.150		0.000	0.000	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.080		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.020		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

All measurements are in g/210L

Estimation of Uncertainty of Measurement and traceability records are located within the Breath Alcohol Section

DFS Technician

[Signature]

Date

11/19/14

Issuing Analyst

[Signature]

Date

11/19/14

jpd

TLN



COMMONWEALTH OF VIRGINIA
DEPARTMENT OF FORENSIC SCIENCE

CERTIFICATE OF BLOOD ALCOHOL ANALYSIS
AS DETERMINED BY A CHEMICAL TEST OF THE ACCUSED'S BREATH

NAME OF ACCUSED INSTRUMENT, TEST,	NAME OF COURT DFS
---	-----------------------------

BREATH ANALYSIS

SAMPLE EXAMINED AND TEST CONDUCTED BY NEECE, JR., TIMMY, L.		AGENCY DFS Central Lab
DFS LICENSE NUMBER 25387	LICENSE EXPIRES 10/01/2016	DATE TEST CONDUCTED 11/19/2014
TEST EQUIPMENT NUMBER 010537		

RESULTS: TIME SAMPLE TAKEN 10:19 EST

SAMPLE'S ALCOHOL CONTENT 0.00 GRAMS PER 210 LITERS OF BREATH

ATTEST:

I CERTIFY THAT THE ABOVE IS AN ACCURATE RECORD OF THE TEST CONDUCTED; THAT THE TEST WAS CONDUCTED WITH THE TYPE OF EQUIPMENT AND IN ACCORDANCE WITH THE METHODS APPROVED BY THE DEPARTMENT OF FORENSIC SCIENCE; THAT THE TEST WAS CONDUCTED IN ACCORDANCE WITH THE DEPARTMENT'S SPECIFICATIONS; THAT PRIOR TO ADMINISTRATION OF THE TEST THE ACCUSED WAS ADVISED OF HIS RIGHT TO OBSERVE THE PROCESS AND SEE THE BLOOD ALCOHOL READING ON THE EQUIPMENT USED TO PERFORM THE BREATH TEST, AND THAT I POSSESS A VALID LICENSE TO CONDUCT SUCH TEST, GIVEN UNDER MY HAND THIS _____ DAY OF _____, 20_____.

BREATH TEST OPERATOR

I HAVE RECEIVED A COPY OF THIS CERTIFICATE OF ANALYSIS _____ SUBJECT'S SIGNATURE

SUBJECT REFUSED TO SIGN FOR COPY OF CERTIFICATE OF ANALYSIS _____ OPERATOR'S SIGNATURE



IntoxNet MIS Report
Report Generated 19 Nov 2014 at 10:48

mmxB
TLW

Test Results

Instrument Serial Number 010537

Test # 001533 Subject Test

Test Location 1 Department of
Test Date 19 Nov 2014

Test Location 2 Forensic Science
Test Time 10:13
Remote/Local Local

Test Location 3
System Check Passed

Operator's Last Name NEECE,JR.
Agency DFS Central Lab

Operator's First Name TIMMY

Operator's Middle Initial L

Card Serial Number 125387

Effective Date 10/01/2014

License Number 25387

Expiration Date 10/01/2016

Subject's Last Name INSTRUMENT

Subject's First Name TEST

Subject's Middle Initial

Subject's Date of Birth 00/00/0000

Subject's Sex Male

Driver's License Number

Driver's License Expiration 00/00/0000

Driver's License State

Court Name DFS

End Date 19 Nov 2014 End Time 10:21

Result Time 10:19

Result Date 19 Nov 2014 Result 0.00

Data Type DIAG

Sample Value Pass

Sample Time 10:14

Data Type BLK

Sample Value 0.000

Sample Time 10:14

Data Type CHK

Sample Value 0.102

Sample Time 10:15

Data Type BLK

Sample Value 0.000

Sample Time 10:16

Data Type SUBJ

Sample Value 0.000

Sample Time 10:17

Data Type BLK

Sample Value 0.000

Sample Time 10:18

Data Type SUBJ

Sample Value 0.000

Sample Time 10:19

Data Type BLK

Sample Value 0.000

Sample Time 10:20

Standard Type Dry Gas Std

Standard Value 0.101

Standard Lot Number AG320502-04

Standard Expiration Date 07/24/2015

Tank Pressure 512

Barometric Pressure 764 mmHg

Blow Sample Number 1 Blow Duration 2.36 sec

Blow Volume 1761 cc End-of-Blow Time 10:17

Blow Sample Number 2 Blow Duration 2.82 sec

Blow Volume 2166 cc End-of-Blow Time 10:19

Tamper Evident Stamp b46e61df

Test Status Code 0

Test Status Success

TLN

Intox EC/IR-II: Accuracy Check

Department of Forensic Science

Serial Number: 010537 Test Number: 1534

Test Date: 11/19/2014 Test Time: 10:22 EST

Dry Gas Target: 0.101

Lot Number: AG320502-04 Exp Date: 07/24/2015

Tank Pressure: 507 psi Barometric Pressure: 764 mmHg

System Check: *Passed*

Test	g/210L	Time
BLK	0.000	10:22
CHK	0.102	10:23
BLK	0.000	10:25
CHK	0.102	10:26
BLK	0.000	10:27
CHK	0.102	10:28

Test Status: *Success*

Calibration CRC: 6B8E7224

TW

Intox EC/IR-II: Accuracy Check

Department of Forensic Science

Serial Number: 010537 Test Number: 1535

Test Date: 11/19/2014 Test Time: 10:30 EST

Dry Gas Target: 0.302

Lot Number: AG428003-10 Exp Date: 10/07/2016

Tank Pressure: 473 psi Barometric Pressure: 765 mmHg

System Check: *Passed*

Test	g/210L	Time
BLK	0.000	10:31
CHK	0.308	10:32
BLK	0.000	10:34
CHK	0.308	10:34
BLK	0.000	10:36
CHK	0.307	10:37

Test Status: *Success*

Calibration CRC: 6B8E7224