

TLN

**Department of Forensic Science
Breath Alcohol Section
Instrument Location History
1/1/1990 To 11/19/2014**

Instrument Serial Number: 010615

As of 19-Nov-14

Start Date	End Date	Agency Name
19-Nov-14		DFS Central Lab
12-Jun-14	19-Nov-14	Charles City County SO
05-Feb-13	12-Jun-14	DFS Central Lab
23-Jan-13	05-Feb-13	New River Valley Regional Jail
09-Aug-12	23-Jan-13	DFS Central Lab
01-Apr-09	09-Aug-12	Carroll County SO
06-Mar-09	01-Apr-09	DFS Central Lab
14-Jan-09	06-Mar-09	Colonial Beach PD
15-Aug-08	14-Jan-09	DFS Central Lab

TW

INTOX EC/IR II Quality Assurance Worksheet

Instrument Serial Number 010615 Worksheet Start Date 11/19/2014
 Location Charles City County SO
 Address 10600 Courthouse Rd Charles City VA 23030
 DFS Technician Timmy Neece, Jr. License No. 25387

Laboratory On-Site

Site Specification: No detrimental environmental conditions exist.

Instrument Barometer (mm HG) 769 Reference Barometer (mm HG) 771

Reference Barometer(RB)Serial # 009111 RB Calibration Due 5/19/2015

Measurement Assurance Check

Standard (sea level)	PA Target	minimum	maximum	Sample 1	0.312
0.300	0.304	0.294	0.313	Sample 2	0.312
Precision		sample min	sample max	Sample 3	0.311
0.001		0.311	0.312		

Standard (sea level)	PA Target	minimum	maximum	Sample 1	0.103
0.100	0.101	0.097	0.104	Sample 2	0.103
Precision		sample min	sample max	Sample 3	0.103
0		0.103	0.103		

Dry gas standard Lot No. (with tank no.) AG400202-33

Replaced dry gas standard (+O-ring)


Installed at Location

Removed to DFS-Central

Supplies
Mouthpieces
Certificates of Analysis
Operator Worksheet
Other:



Notes:

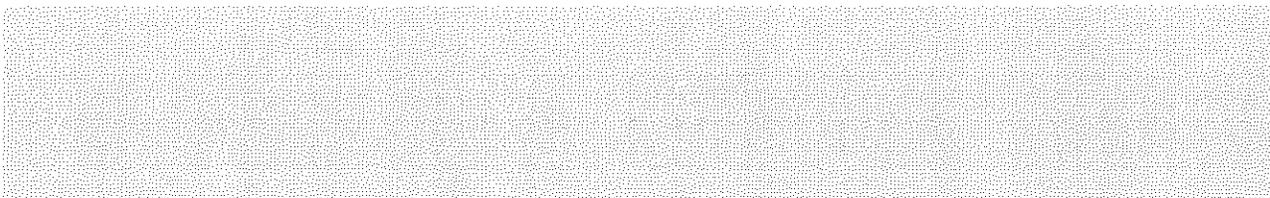

Instrument Serial Number

010615

Certification Date

Calibrated

Certified

Measurement Assurance Check

Instrument Test

Troubleshooting/Maintenance Worksheet Completed

(Successful completion denotes satisfactory condition of the item.)

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.250		0.000	0.000	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.150		0.000	0.000	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.080		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.020		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

All measurements are in g/210L

Estimation of Uncertainty of Measurement and traceability records are located within the Breath Alcohol Section

DFS Technician

Date

11/19/14

Issuing Analyst

Date

11/19/14

JPD

TLN



COMMONWEALTH OF VIRGINIA
DEPARTMENT OF FORENSIC SCIENCE

CERTIFICATE OF BLOOD ALCOHOL ANALYSIS
AS DETERMINED BY A CHEMICAL TEST OF THE ACCUSED'S BREATH

NAME OF ACCUSED INSTRUMENT, TEST,	NAME OF COURT DFS
---	-----------------------------

BREATH ANALYSIS

SAMPLE EXAMINED AND TEST CONDUCTED BY NEECE, JR., TIMMY, L		AGENCY DFS Central Lab
DFS LICENSE NUMBER 25387	LICENSE EXPIRES 10/01/2016	DATE TEST CONDUCTED 11/19/2014
TEST EQUIPMENT NUMBER 010615		

RESULTS: TIME SAMPLE TAKEN 08:26 EST

SAMPLE'S ALCOHOL CONTENT 0.00 GRAMS PER 210 LITERS OF BREATH

ATTEST:

I CERTIFY THAT THE ABOVE IS AN ACCURATE RECORD OF THE TEST CONDUCTED; THAT THE TEST WAS CONDUCTED WITH THE TYPE OF EQUIPMENT AND IN ACCORDANCE WITH THE METHODS APPROVED BY THE DEPARTMENT OF FORENSIC SCIENCE; THAT THE TEST WAS CONDUCTED IN ACCORDANCE WITH THE DEPARTMENT'S SPECIFICATIONS; THAT PRIOR TO ADMINISTRATION OF THE TEST THE ACCUSED WAS ADVISED OF HIS RIGHT TO OBSERVE THE PROCESS AND SEE THE BLOOD ALCOHOL READING ON THE EQUIPMENT USED TO PERFORM THE BREATH TEST, AND THAT I POSSESS A VALID LICENSE TO CONDUCT SUCH TEST, GIVEN UNDER MY HAND THIS _____ DAY OF _____, 20_____.

BREATH TEST OPERATOR

I HAVE RECEIVED A COPY OF THIS CERTIFICATE OF ANALYSIS _____ SUBJECT'S SIGNATURE

SUBJECT REFUSED TO SIGN FOR COPY OF CERTIFICATE OF ANALYSIS _____ OPERATOR'S SIGNATURE

FOR COURT



IntoxNet MIS Report

Report Generated 19 Nov 2014 at 08:57

*MMB
-LW*

Test Results

Instrument Serial Number 010615

Test # 000718 Subject Test

Test Location 1 Department of
 Test Date 19 Nov 2014

Test Location 2 Forensic Science
 Test Time 08:20
 Remote/Local Local

Test Location 3
 System Check Passed

Operator's Last Name NEECE, JR.
 Agency DFS Central Lab

Operator's First Name TIMMY

Operator's Middle Initial L

Card Serial Number 125387
Subject's Last Name INSTRUMENT
Subject's Middle Initial

Effective Date 10/01/2014

License Number 25387

Expiration Date 10/01/2016

Driver's License Number

Subject's Date of Birth 00/00/0000

Subject's First Name TEST

Subject's Sex Male

Driver's License Expiration 00/00/0000

Driver's License State

Court Name DFS

End Date 19 Nov 2014 End Time 08:28

Result Time 08:26

Result Date 19 Nov 2014 Result 0.00

Data Type DIAG

Sample Value Pass

Sample Time 08:20

Data Type BLK

Sample Value 0.000

Sample Time 08:21

Data Type CHK

Sample Value 0.104

Sample Time 08:22

Data Type BLK

Sample Value 0.000

Sample Time 08:23

Data Type SUBJ

Sample Value 0.000

Sample Time 08:24

Data Type BLK

Sample Value 0.000

Sample Time 08:25

Data Type SUBJ

Sample Value 0.000

Sample Time 08:26

Data Type BLK

Sample Value 0.000

Sample Time 08:27

Standard Type Dry Gas Std

Standard Value 0.101

Standard Lot Number AG400202-33

Standard Expiration Date 01/02/2016

Tank Pressure 213

Barometric Pressure 769 mmHg

Blow Sample Number 1 Blow Duration 3.31 sec

Blow Volume 1756 cc End-of-Blow Time 08:24

Blow Sample Number 2 Blow Duration 3.65 sec

Blow Volume 1779 cc End-of-Blow Time 08:26

Tamper Evident Stamp 5de3b0b6

Test Status Code 0

Test Status Success

TLN

Intox EC/IR-II: Accuracy Check

Department of Forensic Science

Serial Number: 010615 Test Number: 719

Test Date: 11/19/2014 Test Time: 08:30 EST

Dry Gas Target: 0.101

Lot Number: AG400202-33 Exp Date: 01/02/2016

Tank Pressure: 208 psi Barometric Pressure: 769 mmHg

System Check: *Passed*

Test	g/210L	Time
BLK	0.000	08:30
CHK	0.103	08:31
BLK	0.000	08:33
CHK	0.103	08:33
BLK	0.000	08:35
CHK	0.103	08:35

Test Status: *Success*

Calibration CRC: 727F0A58

TLN

Intox EC/IR-II: Accuracy Check

Department of Forensic Science

Serial Number: 010615 Test Number: 720

Test Date: 11/19/2014 Test Time: 08:39 EST

Dry Gas Target: 0.304

Lot Number: AG428003-10 Exp Date: 10/07/2016

Tank Pressure: 473 psi Barometric Pressure: 769 mmHg

System Check: *Passed*

Test	g/210L	Time
BLK	0.000	08:39
CHK	0.312	08:40
BLK	0.000	08:42
CHK	0.312	08:43
BLK	0.000	08:44
CHK	0.311	08:45

Test Status: *Success*

Calibration CRC: 727F0A58