

TLN

**Department of Forensic Science
Breath Alcohol Section
Instrument Location History
1/1/1990 To 12/3/2014**

Instrument Serial Number: 010502

As of 03-Dec-14

Start Date	End Date	Agency Name
02-Dec-14		DFS Central Lab
25-Jun-14	02-Dec-14	Northumberland County SO
10-Jun-14	25-Jun-14	DFS Central Lab
16-Nov-11	10-Jun-14	Petersburg PD
09-Nov-11	16-Nov-11	DFS Central Lab
18-Dec-08	09-Nov-11	Petersburg PD
19-May-08	18-Dec-08	DFS Central Lab

TLW

INTOX EC/IR II Quality Assurance Worksheet

Instrument Serial Number **010502** Worksheet Start Date **12/2/2014**
 Location **Northumberland Co SO**
 Address **76 Judicial Place Heathsville VA 22473**
 DFS Technician **Timmy Neece, Jr** License No. **25387**

Laboratory On-Site

Site Specification: No detrimental environmental conditions exist.

Instrument Barometer (mm HG) **772** Reference Barometer (mm HG) **771**
 Reference Barometer(RB)Serial # **009111** RB Calibration Due **5/19/2015**

Measurement Assurance Check


Standard (sea level)	PA Target	minimum	maximum	Sample 1	0.311
0.300	0.304	0.294	0.313	Sample 2	0.311
Precision		sample min	sample max	Sample 3	0.310
0.001		0.310	0.311		

Standard (sea level)	PA Target	minimum	maximum	Sample 1	0.103
0.100	0.101	0.097	0.104	Sample 2	0.103
Precision		sample min	sample max	Sample 3	0.103
0		0.103	0.103		


Dry gas standard Lot No. (with tank no.) **AG332301-26**

- Replaced dry gas standard (+O-ring)
- Installed at Location
- Removed to DFS-Central

Supplies
 Mouthpieces
 Certificates of Analysis
 Operator Worksheet
 Other:



Notes:

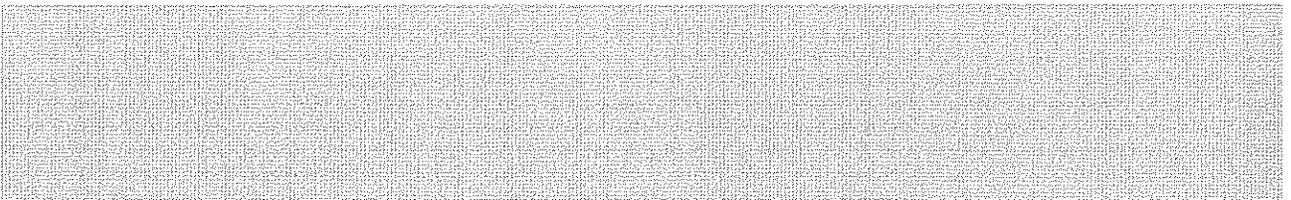

Instrument Serial Number

010502

Certification Date

Calibrated

Certified

Measurement Assurance Check

Instrument Test

Troubleshooting/Maintenance Worksheet Completed

(Successful completion denotes satisfactory condition of the item.)

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.250		0.000	0.000	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.150		0.000	0.000	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.080		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.020		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

All measurements are in g/210L

Estimation of Uncertainty of Measurement and traceability records are located within the Breath Alcohol Section

DFS Technician

[Signature]

Date

12/3/14

Issuing Analyst

[Signature]

Date

12/3/14

JPD

TLN



COMMONWEALTH OF VIRGINIA
DEPARTMENT OF FORENSIC SCIENCE

CERTIFICATE OF BLOOD ALCOHOL ANALYSIS
AS DETERMINED BY A CHEMICAL TEST OF THE ACCUSED'S BREATH

NAME OF ACCUSED INSTRUMENT, TEST,	NAME OF COURT DFS
---	-----------------------------

BREATH ANALYSIS

SAMPLE EXAMINED AND TEST CONDUCTED BY NEECE, JR., TIMMY, L		AGENCY DFS Central Lab
DFS LICENSE NUMBER 25387	LICENSE EXPIRES 10/01/2016	DATE TEST CONDUCTED 12/02/2014
TEST EQUIPMENT NUMBER 010502		

RESULTS: TIME SAMPLE TAKEN 12:30 EST

SAMPLE'S ALCOHOL CONTENT 0.00 GRAMS PER 210 LITERS OF BREATH

ATTEST:

I CERTIFY THAT THE ABOVE IS AN ACCURATE RECORD OF THE TEST CONDUCTED; THAT THE TEST WAS CONDUCTED WITH THE TYPE OF EQUIPMENT AND IN ACCORDANCE WITH THE METHODS APPROVED BY THE DEPARTMENT OF FORENSIC SCIENCE; THAT THE TEST WAS CONDUCTED IN ACCORDANCE WITH THE DEPARTMENT'S SPECIFICATIONS; THAT PRIOR TO ADMINISTRATION OF THE TEST THE ACCUSED WAS ADVISED OF HIS RIGHT TO OBSERVE THE PROCESS AND SEE THE BLOOD ALCOHOL READING ON THE EQUIPMENT USED TO PERFORM THE BREATH TEST, AND THAT I POSSESS A VALID LICENSE TO CONDUCT SUCH TEST, GIVEN UNDER MY HAND THIS _____ DAY OF _____, 20_____.

BREATH TEST OPERATOR

I HAVE RECEIVED A COPY OF THIS CERTIFICATE OF ANALYSIS _____ SUBJECT'S SIGNATURE

SUBJECT REFUSED TO SIGN FOR COPY OF CERTIFICATE OF ANALYSIS _____ OPERATOR'S SIGNATURE



IntoxNet MIS Report

Report Generated 02 Dec 2014 at 12:56

TLW

Test Results

Instrument Serial Number 010502

Test # 000867 Subject Test

Test Location 1 Department of
Test Date 02 Dec 2014

Test Location 2 Forensic Science
Test Time 12:24
Remote/Local Local

Test Location 3
System Check Passed

Operator's Last Name NEECE, JR.
Agency DFS Central Lab

Operator's First Name TIMMY

Operator's Middle Initial L

Card Serial Number 125387

License Number 25387

Effective Date 10/01/2014

Expiration Date 10/01/2016

Subject's Last Name INSTRUMENT

Subject's First Name TEST

Subject's Middle Initial

Subject's Date of Birth 00/00/0000

Subject's Sex Male

Driver's License Number

Driver's License Expiration 00/00/0000

Driver's License State

Court Name DFS

End Date 02 Dec 2014 End Time 12:31

Result Time 12:30

Result Date 02 Dec 2014 Result 0.00

Data Type DIAG

Sample Value Pass

Sample Time 12:24

Data Type BLK

Sample Value 0.000

Sample Time 12:25

Data Type CHK

Sample Value 0.103

Sample Time 12:26

Data Type BLK

Sample Value 0.000

Sample Time 12:27

Data Type SUBJ

Sample Value 0.000

Sample Time 12:28

Data Type BLK

Sample Value 0.000

Sample Time 12:29

Data Type SUBJ

Sample Value 0.000

Sample Time 12:30

Data Type BLK

Sample Value 0.000

Sample Time 12:31

Standard Type Dry Gas Std

Standard Value 0.102

Standard Lot Number AG332301-26

Standard Expiration Date 11/19/2015

Tank Pressure 865

Barometric Pressure 772 mmHg

Blow Sample Number 1 Blow Duration 3.26 sec

Blow Volume 2131 cc End-of-Blow Time 12:28

Blow Sample Number 2 Blow Duration 3.42 sec

Blow Volume 2517 cc End-of-Blow Time 12:30

Tamper Evident Stamp ffa269e9

Test Status Code 0

Test Status Success

TLN

Intox EC/IR-II: Accuracy Check

Department of Forensic Science

Serial Number: 010502 Test Number: 868

Test Date: 12/02/2014 Test Time: 12:34 EST

Dry Gas Target: 0.101

Lot Number: AG332301-26 Exp Date: 11/19/2015

Tank Pressure: 860 psi Barometric Pressure: 771 mmHg

System Check: *Passed*

Test	g/210L	Time
BLK	0.000	12:34
CHK	0.103	12:35
BLK	0.000	12:37
CHK	0.103	12:37
BLK	0.000	12:39
CHK	0.103	12:40

Test Status: *Success*

Calibration CRC: C5BC74FA

TLN

Intox EC/IR-II: Accuracy Check

Department of Forensic Science

Serial Number: 010502 Test Number: 869

Test Date: 12/02/2014 Test Time: 12:42 EST

Dry Gas Target: 0.304

Lot Number: AG428003-03 Exp Date: 10/07/2016

Tank Pressure: 541 psi Barometric Pressure: 771 mmHg

System Check: *Passed*

Test	g/210L	Time
BLK	0.000	12:43
CHK	0.311	12:44
BLK	0.000	12:46
CHK	0.311	12:46
BLK	0.000	12:48
CHK	0.310	12:49

Test Status: *Success*

Calibration CRC: C5BC74FA