

Department of Forensic Science  
Breath Alcohol Section  
Instrument Location History  
1/1/1990 To 11/19/2014

DOH  
Jrd

---

Instrument Serial Number: 010622 As of 19-Nov-14

---

Start Date	End Date	Agency Name
19-Nov-14		DFS Central Lab
11-Jun-14	19-Nov-14	Hopewell PD
29-May-14	11-Jun-14	DFS Central Lab
12-Dec-08	29-May-14	Campbell County SO
04-Aug-08	12-Dec-08	DFS Central Lab

DBH  
fid

# INTOX EC/IR II Quality Assurance Worksheet

Instrument Serial Number 010622 Worksheet Start Date 11/19/2014  
Location Riverside Regional Jail  
Address 1000 River Rd Hopewell VA 23860  
DFS Technician Donald Hall License No. 21250

Laboratory  On-Site

Site Specification: No detrimental environmental conditions exist.

Instrument Barometer (mm HG) 768 Reference Barometer (mm HG) 769  
Reference Barometer(RB)Serial # 009109 RB Calibration Due 7/28/2015

### Measurement Assurance Check

<b>Standard (sea level)</b>	<b>PA Target</b>	<b>minimum</b>	<b>maximum</b>	<b>Sample 1</b>	0.308
0.300	0.303	0.293	0.312	<b>Sample 2</b>	0.307
<b>Precision</b>		<b>sample min</b>	<b>sample max</b>	<b>Sample 3</b>	0.307
0.001		0.307	0.308		

<b>Standard (sea level)</b>	<b>PA Target</b>	<b>minimum</b>	<b>maximum</b>	<b>Sample 1</b>	0.102
0.100	0.101	0.097	0.104	<b>Sample 2</b>	0.102
<b>Precision</b>		<b>sample min</b>	<b>sample max</b>	<b>Sample 3</b>	0.102
0		0.102	0.102		


Dry gas standard Lot No. (with tank no.) AG316301-16

- Replaced dry gas standard (+O-ring)
- Installed at Location
- Removed to DFS-Central

Supplies  
Mouthpieces  
Certificates of Analysis  
Operator Worksheet  
Other:



Notes:

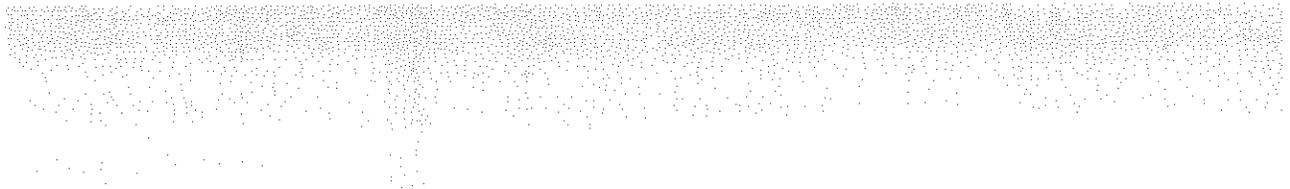

Instrument Serial Number

010622

Certification Date

Calibrated

Certified

Measurement Assurance Check

Instrument Test

Troubleshooting/Maintenance Worksheet Completed

(Successful completion denotes satisfactory condition of the item.)

<b>Standard (sea level)</b>	<b>PA Target</b>	<b>minimum</b>	<b>maximum</b>	<b>Sample 1</b>
0.250		0.000	0.000	<b>Sample 2</b>
<b>Precision</b>		<b>sample min</b>	<b>sample max</b>	<b>Sample 3</b>
0		0.000	0.000	

<b>Standard (sea level)</b>	<b>PA Target</b>	<b>minimum</b>	<b>maximum</b>	<b>Sample 1</b>
0.150		0.000	0.000	<b>Sample 2</b>
<b>Precision</b>		<b>sample min</b>	<b>sample max</b>	<b>Sample 3</b>
0		0.000	0.000	

<b>Standard (sea level)</b>	<b>PA Target</b>	<b>minimum</b>	<b>maximum</b>	<b>Sample 1</b>
0.080		-0.003	0.003	<b>Sample 2</b>
<b>Precision</b>		<b>sample min</b>	<b>sample max</b>	<b>Sample 3</b>
0		0.000	0.000	

<b>Standard (sea level)</b>	<b>PA Target</b>	<b>minimum</b>	<b>maximum</b>	<b>Sample 1</b>
0.020		-0.003	0.003	<b>Sample 2</b>
<b>Precision</b>		<b>sample min</b>	<b>sample max</b>	<b>Sample 3</b>
0		0.000	0.000	

All measurements are in g/210L

Estimation of Uncertainty of Measurement and traceability records are located within the Breath Alcohol Section

DFS Technician Donald B Hall Date 11/19/14

Issuing Analyst [Signature] Date 11/20/14

JPD

18H  
fd



COMMONWEALTH OF VIRGINIA  
DEPARTMENT OF FORENSIC SCIENCE

CERTIFICATE OF BLOOD ALCOHOL ANALYSIS  
AS DETERMINED BY A CHEMICAL TEST OF THE ACCUSED'S BREATH

NAME OF ACCUSED  <b>INSTRUMENT, TEST,</b>	NAME OF COURT  <b>DFS</b>
---	---------------------------------

**BREATH ANALYSIS**

SAMPLE EXAMINED AND TEST CONDUCTED BY  <b>HALL, DONALD, B</b>		AGENCY  <b>DFS Central Lab</b>
DFS LICENSE NUMBER  <b>21250</b>	LICENSE EXPIRES  <b>10/01/2016</b>	DATE TEST CONDUCTED  <b>11/19/2014</b>
TEST EQUIPMENT NUMBER  <b>010622</b>		

RESULTS: TIME SAMPLE TAKEN 11:18 EST

SAMPLE'S ALCOHOL CONTENT 0.00 GRAMS PER 210 LITERS OF BREATH

**ATTEST:**

I CERTIFY THAT THE ABOVE IS AN ACCURATE RECORD OF THE TEST CONDUCTED; THAT THE TEST WAS CONDUCTED WITH THE TYPE OF EQUIPMENT AND IN ACCORDANCE WITH THE METHODS APPROVED BY THE DEPARTMENT OF FORENSIC SCIENCE; THAT THE TEST WAS CONDUCTED IN ACCORDANCE WITH THE DEPARTMENT'S SPECIFICATIONS; THAT PRIOR TO ADMINISTRATION OF THE TEST THE ACCUSED WAS ADVISED OF HIS RIGHT TO OBSERVE THE PROCESS AND SEE THE BLOOD ALCOHOL READING ON THE EQUIPMENT USED TO PERFORM THE BREATH TEST, AND THAT I POSSESS A VALID LICENSE TO CONDUCT SUCH TEST, GIVEN UNDER MY HAND THIS \_\_\_\_\_ DAY OF \_\_\_\_\_, 20 \_\_\_\_\_.

BREATH TEST OPERATOR
----------------------

I HAVE RECEIVED A COPY OF THIS CERTIFICATE OF ANALYSIS \_\_\_\_\_ SUBJECT'S SIGNATURE

SUBJECT REFUSED TO SIGN FOR COPY OF CERTIFICATE OF ANALYSIS \_\_\_\_\_ OPERATOR'S SIGNATURE



# IntoxNet MIS Report

Report Generated 19 Nov 2014 at 11:55

*id*  
*DBH*  
*Sid*

## Test Results

**Instrument Serial Number 010622**

**Test # 001251 Subject Test**

Test Location 1 Department of  
Test Date 19 Nov 2014

Test Location 2 Forensic Science  
Test Time 11:11  
Remote/Local Local

Test Location 3  
System Check Passed

Operator's Last Name HALL  
Agency DFS Central Lab

Operator's First Name DONALD

Operator's Middle Initial B

Card Serial Number 121250

License Number 21250

Effective Date 10/01/2014

Expiration Date 10/01/2016

Subject's Last Name INSTRUMENT

Subject's First Name TEST

Subject's Middle Initial

Subject's Date of Birth 00/00/0000

Subject's Sex Male

Driver's License Number

Driver's License Expiration 00/00/0000

Driver's License State

Court Name DFS

End Date 19 Nov 2014 End Time 11:19

Result Time 11:18

Result Date 19 Nov 2014 Result 0.00

Data Type DIAG

Sample Value Pass

Sample Time 11:12

Data Type BLK

Sample Value 0.000

Sample Time 11:12

Data Type CHK

Sample Value 0.102

Sample Time 11:13

Data Type BLK

Sample Value 0.000

Sample Time 11:14

Data Type SUBJ

Sample Value 0.000

Sample Time 11:15

Data Type BLK

Sample Value 0.000

Sample Time 11:16

Data Type SUBJ

Sample Value 0.000

Sample Time 11:18

Data Type BLK

Sample Value 0.000

Sample Time 11:19

Standard Type Dry Gas Std

Standard Value 0.101

Standard Lot Number AG316301-16

Standard Expiration Date 06/12/2015

Tank Pressure 580

Barometric Pressure 768 mmHg

Blow Sample Number 1 Blow Duration 3.56 sec

Blow Volume 1955 cc End-of-Blow Time 11:15

Blow Sample Number 2 Blow Duration 3.83 sec

Blow Volume 2015 cc End-of-Blow Time 11:18

Tamper Evident Stamp 62e1cb57

Test Status Code 0

Test Status Success

DBF.

**Intox EC/1R-11: Accuracy Check**

*sd*

*Department of Forensic Science*

Serial Number: 010622      Test Number: 1252

Test Date: 11/19/2014      Test Time: 11:20 EST

Dry Gas Target: 0.101

Lot Number: AG316301-16      Exp Date: 06/12/2015

Tank Pressure: 575 psi      Barometric Pressure: 767 mmHg

System Check: *Passed*

Test	g/210L	Time
BLK	0.000	11:21
CHK	0.102	11:22
BLK	0.000	11:23
CHK	0.102	11:24
BLK	0.000	11:25
CHK	0.102	11:26

Test Status: *Success*

Calibration CRC: BF7A46B5

DBH  
PCL

**Intox EC/IR-11: Accuracy Check**

*Department of Forensic Science*

Serial Number: 010622      Test Number: 1253  
Test Date: 11/19/2014      Test Time: 11:29 EST  
Dry Gas Target: 0.303

Lot Number: AG421201-03      Exp Date: 07/31/2016  
Tank Pressure: 178 psi      Barometric Pressure: 767 mmHg  
System Check: *Passed*

Test	g/210L	Time
BLK	0.000	11:30
CHK	0.308	11:30
BLK	0.000	11:32
CHK	0.307	11:33
BLK	0.000	11:35
CHK	0.307	11:36

Test Status: *Success*

Calibration CRC: BF7A46B5