

Department of Forensic Science  
Breath Alcohol Section  
Instrument Location History  
1/1/1990 To 1/7/2015

*HHS*  
*ful*

**Instrument Serial Number: 010505**

**As of 07-Jan-15**

<b>Start Date</b>	<b>End Date</b>	<b>Agency Name</b>
07-Jan-15		DFS Central Lab
30-Jul-14	07-Jan-15	Sussex County SO
18-Jun-14	30-Jul-14	DFS Central Lab
11-Dec-08	18-Jun-14	Chincoteague PD
02-Jun-08	11-Dec-08	DFS Central Lab

# INTOX EC/IR II Quality Assurance Worksheet

*HMS*  
*EW*

Instrument Serial Number: 010505      Worksheet Start Date: 1/7/2015

Location: Sussex County

Address: 20212 Thornton Sq., Sussex, VA 23884

DFS Technician: Heather Stanton      License No.: 18910

Laboratory       On-Site

Site Specification: No detrimental environmental conditions exist.

Instrument Barometer (mm HG): 759      Reference Barometer (mm HG): 761

Reference Barometer(RB)Serial #: 009113      RB Calibration Due: 4/28/2015

**Measurement Assurance Check**


<b>Standard (sea level)</b>	0.300	<b>PA Target</b>	0.300	<b>minimum</b>	0.291	<b>maximum</b>	0.309	<b>Sample 1</b>	0.302
<b>Precision</b>	0.001			<b>sample min</b>	0.301	<b>sample max</b>	0.302	<b>Sample 2</b>	0.301
								<b>Sample 3</b>	0.301

<b>Standard (sea level)</b>	0.100	<b>PA Target</b>	0.100	<b>minimum</b>	0.097	<b>maximum</b>	0.103	<b>Sample 1</b>	0.099
<b>Precision</b>	0			<b>sample min</b>	0.099	<b>sample max</b>	0.099	<b>Sample 2</b>	0.099
								<b>Sample 3</b>	0.099

Dry gas standard Lot No. (with tank no.)      AG316301-04

- Replaced dry gas standard (+O-ring)
  - Installed at Location
  - Removed to DFS-Central
- Supplies  
Mouthpieces  
Certificates of Analysis  
Operator Worksheet  
Other:

Notes:

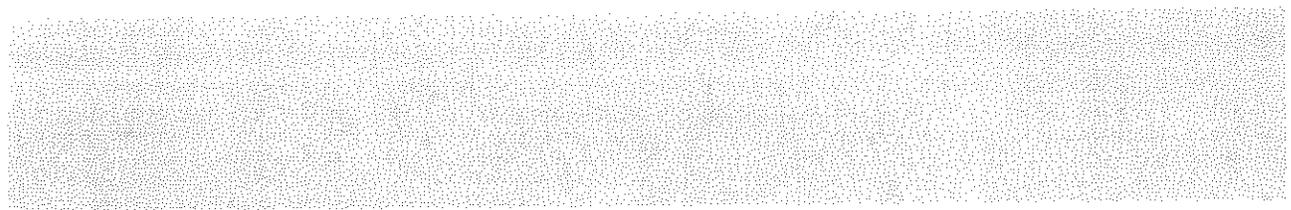

Instrument Serial Number

010505

Certification Date

Calibrated

Certified

Measurement Assurance Check

Instrument Test

Troubleshooting/Maintenance Worksheet Completed

(Successful completion denotes satisfactory condition of the item.)

<b>Standard (sea level)</b>	<b>PA Target</b>	<b>minimum</b>	<b>maximum</b>	<b>Sample 1</b>
0.250		0.000	0.000	<b>Sample 2</b>
<b>Precision</b>		<b>sample min</b>	<b>sample max</b>	<b>Sample 3</b>
0		0.000	0.000	

<b>Standard (sea level)</b>	<b>PA Target</b>	<b>minimum</b>	<b>maximum</b>	<b>Sample 1</b>
0.150		0.000	0.000	<b>Sample 2</b>
<b>Precision</b>		<b>sample min</b>	<b>sample max</b>	<b>Sample 3</b>
0		0.000	0.000	

<b>Standard (sea level)</b>	<b>PA Target</b>	<b>minimum</b>	<b>maximum</b>	<b>Sample 1</b>
0.080		-0.003	0.003	<b>Sample 2</b>
<b>Precision</b>		<b>sample min</b>	<b>sample max</b>	<b>Sample 3</b>
0		0.000	0.000	

<b>Standard (sea level)</b>	<b>PA Target</b>	<b>minimum</b>	<b>maximum</b>	<b>Sample 1</b>
0.020		-0.003	0.003	<b>Sample 2</b>
<b>Precision</b>		<b>sample min</b>	<b>sample max</b>	<b>Sample 3</b>
0		0.000	0.000	

All measurements are in g/210L

Estimation of Uncertainty of Measurement and traceability records are located within the Breath Alcohol Section

DFS Technician

*Heath m Stach*

Date

*1/7/15*

Issuing Analyst

*jud*

Date

*1/12/15*

*JPD*



COMMONWEALTH OF VIRGINIA  
DEPARTMENT OF FORENSIC SCIENCE

*Handwritten initials/signature*

CERTIFICATE OF BLOOD ALCOHOL ANALYSIS  
AS DETERMINED BY A CHEMICAL TEST OF THE ACCUSED'S BREATH

NAME OF ACCUSED <b>INSTRUMENT, TEST,</b>	NAME OF COURT <b>DFS</b>
---	-----------------------------

**BREATH ANALYSIS**

SAMPLE EXAMINED AND TEST CONDUCTED BY <b>STANTON, HEATHER, M</b>		AGENCY <b>DFS Central Lab</b>
DFS LICENSE NUMBER <b>18910</b>	LICENSE EXPIRES <b>10/01/2016</b>	DATE TEST CONDUCTED <b>01/07/2015</b>
TEST EQUIPMENT NUMBER <b>010505</b>		

RESULTS: TIME SAMPLE TAKEN 09:28 EST  
 SAMPLE'S ALCOHOL CONTENT 0.00 GRAMS PER 210 LITERS OF BREATH

**ATTEST:**

I CERTIFY THAT THE ABOVE IS AN ACCURATE RECORD OF THE TEST CONDUCTED; THAT THE TEST WAS CONDUCTED WITH THE TYPE OF EQUIPMENT AND IN ACCORDANCE WITH THE METHODS APPROVED BY THE DEPARTMENT OF FORENSIC SCIENCE; THAT THE TEST WAS CONDUCTED IN ACCORDANCE WITH THE DEPARTMENT'S SPECIFICATIONS; THAT PRIOR TO ADMINISTRATION OF THE TEST THE ACCUSED WAS ADVISED OF HIS RIGHT TO OBSERVE THE PROCESS AND SEE THE BLOOD ALCOHOL READING ON THE EQUIPMENT USED TO PERFORM THE BREATH TEST, AND THAT I POSSESS A VALID LICENSE TO CONDUCT SUCH TEST, GIVEN UNDER MY HAND THIS \_\_\_\_\_ DAY OF \_\_\_\_\_, 20\_\_\_\_\_.

BREATH TEST OPERATOR
----------------------

I HAVE RECEIVED A COPY OF THIS CERTIFICATE OF ANALYSIS \_\_\_\_\_ SUBJECT'S SIGNATURE

SUBJECT REFUSED TO SIGN FOR COPY OF CERTIFICATE OF ANALYSIS \_\_\_\_\_ OPERATOR'S SIGNATURE



# IntoxNet MIS Report

Report Generated 07 Jan 2015 at 14:18

*Handwritten initials/signature*

## Test Results

**Instrument Serial Number 010505**

**Test # 000370**      Subject Test

Test Location 1    Department of  
Test Date    07 Jan 2015

Test Location 2    Forensic Science  
Test Time    09:22  
Remote/Local    Local

Test Location 3  
System Check    Passed

Operator's Last Name    STANTON  
Agency    DFS Central Lab

Operator's First Name    HEATHER

Operator's Middle Initial    M

Card Serial Number    118910

License Number    18910

Effective Date    10/01/2014

Expiration Date    10/01/2016

Subject's Last Name    INSTRUMENT

Subject's First Name    TEST

Subject's Middle Initial

Subject's Date of Birth    00/00/0000

Subject's Sex    Male

Driver's License Number

Driver's License Expiration    00/00/0000

Driver's License State

Court Name    DFS

End Date    07 Jan 2015      End Time    09:29

Result Time    09:28

Result Date    07 Jan 2015

Result    0.00

Data Type    DIAG

Sample Value    Pass

Sample Time    09:22

Data Type    BLK

Sample Value    0.000

Sample Time    09:23

Data Type    CHK

Sample Value    0.100

Sample Time    09:24

Data Type    BLK

Sample Value    0.000

Sample Time    09:25

Data Type    SUBJ

Sample Value    0.000

Sample Time    09:26

Data Type    BLK

Sample Value    0.000

Sample Time    09:27

Data Type    SUBJ

Sample Value    0.000

Sample Time    09:28

Data Type    BLK

Sample Value    0.000

Sample Time    09:29

Standard Type    Dry Gas Std

Standard Value    0.100

Standard Lot Number    AG316301-04

Standard Expiration Date    06/12/2015

Tank Pressure    845

Barometric Pressure    759 mmHg

Blow Sample Number    1      Blow Duration    3.30 sec

Blow Volume    1757 cc      End-of-Blow Time    09:26

Blow Sample Number    2      Blow Duration    3.28 sec

Blow Volume    1720 cc      End-of-Blow Time    09:28

Tamper Evident Stamp    088b2c2b

Test Status Code    0

Test Status    Success

IMS  
fd

**Intox EC/IR-II: Accuracy Check**

*Department of Forensic Science*

Serial Number: 010505      Test Number: 371

Test Date: 01/07/2015      Test Time: 09:30 EST

Dry Gas Target: 0.100

Lot Number: AG316301-04      Exp Date: 06/12/2015

Tank Pressure: 840 psi      Barometric Pressure: 759 mmHg

System Check: *Passed*

Test	g/210L	Time
BLK	0.000	09:31
CHK	0.099	09:32
BLK	0.000	09:34
CHK	0.099	09:34
BLK	0.000	09:36
CHK	0.099	09:36

Test Status: *Success*

Calibration CRC: 5BD468F2

IMS  
RL

**Intox EC/IR-II: Accuracy Check**

*Department of Forensic Science*

Serial Number: 010505      Test Number: 372

Test Date: 01/07/2015      Test Time: 09:39 EST

Dry Gas Target: 0.300

Lot Number: AG428003-09      Exp Date: 10/07/2016

Tank Pressure: 448 psi      Barometric Pressure: 759 mmHg

System Check: *Passed*

Test	q/210L	Time
BLK	0.000	09:40
CHK	0.302	09:41
BLK	0.000	09:43
CHK	0.301	09:43
BLK	0.000	09:45
CHK	0.301	09:46

Test Status: *Success*

Calibration CRC: 5BD468F2