

Department of Forensic Science  
Breath Alcohol Section  
Instrument Location History  
1/1/1990 To 1/23/2015

DBH  
mmB

Instrument Serial Number: 010572

As of 23-Jan-15

Start Date	End Date	Agency Name
22-Jan-15		DFS Central Lab
19-Aug-14	22-Jan-15	Washington County Sheriff's Office
30-Jul-14	19-Aug-14	DFS Central Lab
06-Jan-09	30-Jul-14	Sussex County SO
30-Jun-08	06-Jan-09	DFS Central Lab

DBH  
mmB

# INTOX EC/IR II Quality Assurance Worksheet

Instrument Serial Number **010572** Worksheet Start Date **1/22/2015**  
 Location **Washington CO Jail**  
 Address **15205 Joe Derting Dr Abingdon VA 24210**  
 DFS Technician **Donald Hall** License No. **21250**  
 Laboratory  On-Site

Site Specification: No detrimental environmental conditions exist.

Instrument Barometer (mm HG) **711** Reference Barometer (mm HG) **711**  
 Reference Barometer(RB)Serial # **009109** RB Calibration Due **7/28/2015**

### Measurement Assurance Check

<b>Standard (sea level)</b>	<b>PA Target</b>	<b>minimum</b>	<b>maximum</b>	<b>Sample 1</b>	0.284
0.300	0.280	0.271	0.288	<b>Sample 2</b>	0.284
<b>Precision</b>		<b>sample min</b>	<b>sample max</b>	<b>Sample 3</b>	0.284
0		0.284	0.284		

<b>Standard (sea level)</b>	<b>PA Target</b>	<b>minimum</b>	<b>maximum</b>	<b>Sample 1</b>	0.093
0.100	0.094	0.091	0.097	<b>Sample 2</b>	0.093
<b>Precision</b>		<b>sample min</b>	<b>sample max</b>	<b>Sample 3</b>	0.093
0		0.093	0.093		


Dry gas standard Lot No. (with tank no.) **AG419702-41**

- Replaced dry gas standard (+O-ring)
- Installed at Location
- Removed to DFS-Central

Supplies  
 Mouthpieces  
 Certificates of Analysis  
 Operator Worksheet  
 Other:



Notes:

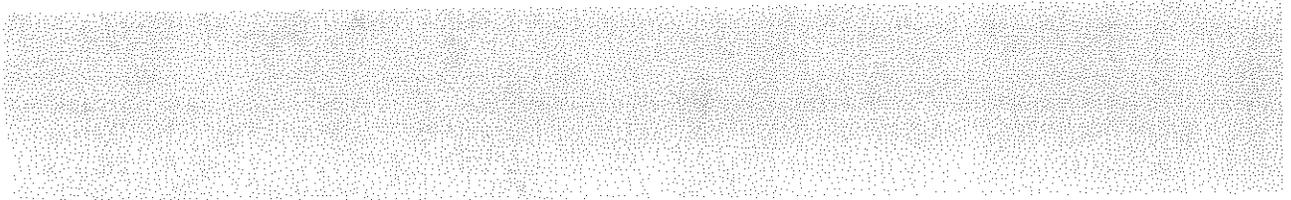

Instrument Serial Number

010572

Certification Date

Calibrated

Certified

Measurement Assurance Check

Instrument Test

Troubleshooting/Maintenance Worksheet Completed

(Successful completion denotes satisfactory condition of the item.)

<b>Standard (sea level)</b>	<b>PA Target</b>	<b>minimum</b>	<b>maximum</b>	<b>Sample 1</b>
0.250		0.000	0.000	<b>Sample 2</b>
<b>Precision</b>		<b>sample min</b>	<b>sample max</b>	<b>Sample 3</b>
0		0.000	0.000	

<b>Standard (sea level)</b>	<b>PA Target</b>	<b>minimum</b>	<b>maximum</b>	<b>Sample 1</b>
0.150		0.000	0.000	<b>Sample 2</b>
<b>Precision</b>		<b>sample min</b>	<b>sample max</b>	<b>Sample 3</b>
0		0.000	0.000	

<b>Standard (sea level)</b>	<b>PA Target</b>	<b>minimum</b>	<b>maximum</b>	<b>Sample 1</b>
0.080		-0.003	0.003	<b>Sample 2</b>
<b>Precision</b>		<b>sample min</b>	<b>sample max</b>	<b>Sample 3</b>
0		0.000	0.000	

<b>Standard (sea level)</b>	<b>PA Target</b>	<b>minimum</b>	<b>maximum</b>	<b>Sample 1</b>
0.020		-0.003	0.003	<b>Sample 2</b>
<b>Precision</b>		<b>sample min</b>	<b>sample max</b>	<b>Sample 3</b>
0		0.000	0.000	

All measurements are in g/210L

Estimation of Uncertainty of Measurement and traceability records are located within the Breath Alcohol Section

DFS Technician

Donald B Hall

Date

1/23/15

Issuing Analyst

Michele Bellini

Date

1/26/15

JPO

DBH  
mmB



COMMONWEALTH OF VIRGINIA  
DEPARTMENT OF FORENSIC SCIENCE

CERTIFICATE OF BLOOD ALCOHOL ANALYSIS  
AS DETERMINED BY A CHEMICAL TEST OF THE ACCUSED'S BREATH

NAME OF ACCUSED  INSTRUMENT, TEST,	NAME OF COURT  DFS
--	--------------------------

BREATH ANALYSIS

SAMPLE EXAMINED AND TEST CONDUCTED BY  HALL, DONALD, B		AGENCY  DFS Central Lab
DFS LICENSE NUMBER  21250	LICENSE EXPIRES  10/01/2016	DATE TEST CONDUCTED  01/22/2015
TEST EQUIPMENT NUMBER  010572		

RESULTS: TIME SAMPLE TAKEN 12:47 EST

SAMPLE'S ALCOHOL CONTENT 0.00 GRAMS PER 210 LITERS OF BREATH

ATTEST:

I CERTIFY THAT THE ABOVE IS AN ACCURATE RECORD OF THE TEST CONDUCTED; THAT THE TEST WAS CONDUCTED WITH THE TYPE OF EQUIPMENT AND IN ACCORDANCE WITH THE METHODS APPROVED BY THE DEPARTMENT OF FORENSIC SCIENCE; THAT THE TEST WAS CONDUCTED IN ACCORDANCE WITH THE DEPARTMENT'S SPECIFICATIONS; THAT PRIOR TO ADMINISTRATION OF THE TEST THE ACCUSED WAS ADVISED OF HIS RIGHT TO OBSERVE THE PROCESS AND SEE THE BLOOD ALCOHOL READING ON THE EQUIPMENT USED TO PERFORM THE BREATH TEST, AND THAT I POSSESS A VALID LICENSE TO CONDUCT SUCH TEST, GIVEN UNDER MY HAND THIS \_\_\_\_\_ DAY OF \_\_\_\_\_, 20\_\_\_\_\_.

BREATH TEST OPERATOR
----------------------

I HAVE RECEIVED A COPY OF THIS CERTIFICATE OF ANALYSIS \_\_\_\_\_ SUBJECT'S SIGNATURE

SUBJECT REFUSED TO SIGN FOR COPY OF CERTIFICATE OF ANALYSIS \_\_\_\_\_ OPERATOR'S SIGNATURE



**IntoxNet MIS Report**  
Report Generated 22 Jan 2015 at 13:23

DBH  
mmB

Test Results

**Instrument Serial Number 010572**

**Test # 000574**      Subject Test

Test Location 1    Department of  
Test Date    22 Jan 2015

Test Location 2    Forensic Science  
Test Time    12:41  
Remote/Local    Local

Test Location 3  
System Check    Passed

Operator's Last Name    HALL  
Agency    DFS Central Lab

Operator's First Name    DONALD

Operator's Middle Initial    B  
License Number    21250

Card Serial Number    121250

Effective Date    10/01/2014

Expiration Date    10/01/2016

Subject's Last Name    INSTRUMENT

Subject's First Name    TEST

Subject's Middle Initial

Subject's Date of Birth    00/00/0000

Subject's Sex    Male

Driver's License Number

Driver's License Expiration    00/00/0000

Driver's License State

Court Name    DFS

End Date    22 Jan 2015      End Time    12:48

Result Time    12:47

Result Date    22 Jan 2015      Result    0.00

Data Type    DIAG

Sample Value    Pass

Sample Time    12:41

Data Type    BLK

Sample Value    0.000

Sample Time    12:42

Data Type    CHK

Sample Value    0.093

Sample Time    12:43

Data Type    BLK

Sample Value    0.000

Sample Time    12:44

Data Type    SUBJ

Sample Value    0.000

Sample Time    12:45

Data Type    BLK

Sample Value    0.000

Sample Time    12:46

Data Type    SUBJ

Sample Value    0.000

Sample Time    12:47

Data Type    BLK

Sample Value    0.000

Sample Time    12:48

Standard Type    Dry Gas Std

Standard Value    0.093

Standard Lot Number    AG419702-41

Standard Expiration Date    07/16/2016

Tank Pressure    1017

Barometric Pressure    710 mmHg

Blow Sample Number    1      Blow Duration    3.99 sec

Blow Volume    2123 cc      End-of-Blow Time    12:45

Blow Sample Number    2      Blow Duration    3.66 sec

Blow Volume    1958 cc      End-of-Blow Time    12:47

Tamper Evident Stamp    3c890564

Test Status Code    0

Test Status    Success

Intox EC/IR-II: Accuracy Check

DH  
mmB

*Department of Forensic Science*

Serial Number: 010572      Test Number: 575

Test Date: 01/22/2015      Test Time: 12:50 EST

Dry Gas Target: 0.094

Lot Number: AG419702-41      Exp Date: 07/16/2016

Tank Pressure: 1007 psi      Barometric Pressure: 711 mmHg

System Check: *Passed*

Test	g/210L	Time
BLK	0.000	12:50
CHK	0.093	12:51
BLK	0.000	12:53
CHK	0.093	12:54
BLK	0.000	12:55
CHK	0.093	12:56

Test Status: *Success*

Calibration CRC: 8E7FA4DC

DBH  
mmB

Intox EC/IR-II: Accuracy Check

Department of Forensic Science

Serial Number: 010572 Test Number: 576

Test Date: 01/22/2015 Test Time: 12:58 EST

Dry Gas Target: 0.280

Lot Number: AG428003-01 Exp Date: 10/07/2016

Tank Pressure: 95 psi Barometric Pressure: 710 mmHg

System Check: Passed

Test	g/210L	Time
BLK	0.000	12:59
CHK	0.284	13:00
BLK	0.000	13:02
CHK	0.284	13:02
BLK	0.000	13:05
CHK	0.284	13:05

Test Status: Success

Calibration CRC: 8E7FA4DC