

Department of Forensic Science
Breath Alcohol Section
Instrument Location History
1/1/1990 To 1/9/2015

Feb

Instrument Serial Number: 010623

As of 09-Jan-15

Start Date	End Date	Agency Name
07-Jan-15		DFS Central Lab
23-Jul-14	07-Jan-15	Colonial Beach PD
26-Jun-14	23-Jul-14	DFS Central Lab
04-Dec-12	26-Jun-14	Fauquier County SO
23-Oct-12	04-Dec-12	DFS Central Lab
06-Aug-09	23-Oct-12	Manassas Park PD
04-Aug-08	06-Aug-09	DFS Central Lab

fid

INTOX EC/IR II Quality Assurance Worksheet

Instrument Serial Number **010623** Worksheet Start Date **1/7/2015**

Location **Colonial Beach Police Department**

Address **907 McKinney Blvd Colonial Beach VA 22443**

DFS Technician **Sarah Dersch** License No. **24178**

Laboratory On-Site

Site Specification: No detrimental environmental conditions exist.

Instrument Barometer (mm HG) **762** Reference Barometer (mm HG) **765**

Reference Barometer(RB)Serial # **009111** RB Calibration Due **5/19/2015**

Measurement Assurance Check

Standard (sea level)	PA Target	minimum	maximum	Sample 1	0.306
0.300	0.301	0.291	0.310	Sample 2	0.306
Precision		sample min	sample max	Sample 3	0.305
0.001		0.305	0.306		

Standard (sea level)	PA Target	minimum	maximum	Sample 1	0.101
0.100	0.100	0.097	0.103	Sample 2	0.101
Precision		sample min	sample max	Sample 3	0.101
0		0.101	0.101		


Dry gas standard Lot No. (with tank no.) **AG316301-23**

- Replaced dry gas standard (+O-ring)
- Installed at Location
- Removed to DFS-Central

Supplies
Mouthpieces
Certificates of Analysis
Operator Worksheet
Other:



Notes:

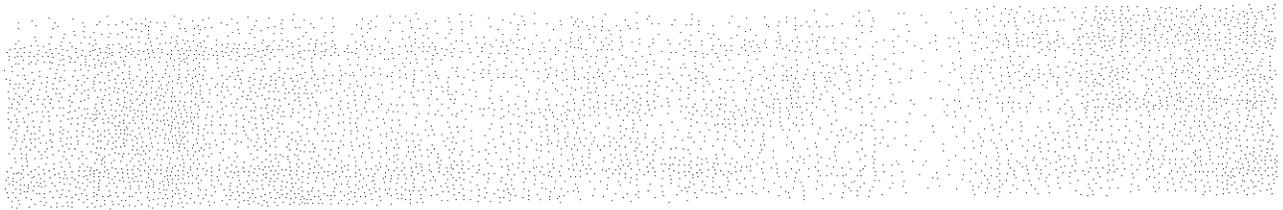

Instrument Serial Number

010623

Certification Date

Calibrated

Certified

Measurement Assurance Check

Instrument Test

Troubleshooting/Maintenance Worksheet Completed

(Successful completion denotes satisfactory condition of the item.)

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.250		0.000	0.000	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.150		0.000	0.000	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	


Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.080		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.020		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

All measurements are in g/210L

Estimation of Uncertainty of Measurement and traceability records are located within the Breath Alcohol Section

DFS Technician

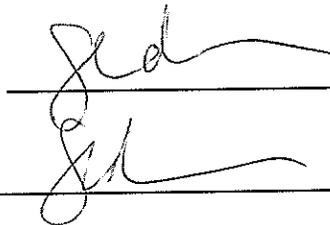

Date

1/9/15

Issuing Analyst



Date

1/9/15

JPD

sl



COMMONWEALTH OF VIRGINIA
DEPARTMENT OF FORENSIC SCIENCE

CERTIFICATE OF BLOOD ALCOHOL ANALYSIS
AS DETERMINED BY A CHEMICAL TEST OF THE ACCUSED'S BREATH

NAME OF ACCUSED INSTRUMENT, TEST,	NAME OF COURT DFS
--	--------------------------

BREATH ANALYSIS

SAMPLE EXAMINED AND TEST CONDUCTED BY DERSCH, SARAH, E		AGENCY DFS Central Lab
DFS LICENSE NUMBER 24178	LICENSE EXPIRES 10/01/2016	DATE TEST CONDUCTED 01/07/2015
TEST EQUIPMENT NUMBER 010623		

RESULTS: TIME SAMPLE TAKEN 12:34 EST

SAMPLE'S ALCOHOL CONTENT 0.00 GRAMS PER 210 LITERS OF BREATH

ATTEST:

I CERTIFY THAT THE ABOVE IS AN ACCURATE RECORD OF THE TEST CONDUCTED; THAT THE TEST WAS CONDUCTED WITH THE TYPE OF EQUIPMENT AND IN ACCORDANCE WITH THE METHODS APPROVED BY THE DEPARTMENT OF FORENSIC SCIENCE; THAT THE TEST WAS CONDUCTED IN ACCORDANCE WITH THE DEPARTMENT'S SPECIFICATIONS; THAT PRIOR TO ADMINISTRATION OF THE TEST THE ACCUSED WAS ADVISED OF HIS RIGHT TO OBSERVE THE PROCESS AND SEE THE BLOOD ALCOHOL READING ON THE EQUIPMENT USED TO PERFORM THE BREATH TEST, AND THAT I POSSESS A VALID LICENSE TO CONDUCT SUCH TEST, GIVEN UNDER MY HAND THIS _____ DAY OF _____, 20_____.

BREATH TEST OPERATOR

I HAVE RECEIVED A COPY OF THIS CERTIFICATE OF ANALYSIS _____ SUBJECT'S SIGNATURE

SUBJECT REFUSED TO SIGN FOR COPY OF CERTIFICATE OF ANALYSIS _____ OPERATOR'S SIGNATURE



IntoxNet MIS Report

Report Generated 09 Jan 2015 at 09:54

Std

Test Results

Instrument Serial Number 010623

Test # 000938 **Subject Test**

Test Location 1 Department of
Test Date 07 Jan 2015

Test Location 2 Forensic Science
Test Time 12:28
Remote/Local Local

Test Location 3
System Check Passed

Operator's Last Name DERSCH
Agency DFS Central Lab

Operator's First Name SARAH

Operator's Middle Initial E

Card Serial Number 124178

Effective Date 10/01/2014

License Number 24178

Expiration Date 10/01/2016

Subject's Last Name INSTRUMENT

Subject's First Name TEST

Subject's Middle Initial

Subject's Date of Birth 00/00/0000

Subject's Sex Male

Driver's License Number

Driver's License Expiration 00/00/0000

Driver's License State

Court Name DFS

End Date 07 Jan 2015 End Time 12:35

Result Time 12:34

Result Date 07 Jan 2015 Result 0.00

Data Type DIAG

Sample Value Pass

Sample Time 12:28

Data Type BLK

Sample Value 0.000

Sample Time 12:29

Data Type CHK

Sample Value 0.102

Sample Time 12:30

Data Type BLK

Sample Value 0.000

Sample Time 12:31

Data Type SUBJ

Sample Value 0.000

Sample Time 12:32

Data Type BLK

Sample Value 0.000

Sample Time 12:33

Data Type SUBJ

Sample Value 0.000

Sample Time 12:34

Data Type BLK

Sample Value 0.000

Sample Time 12:35

Standard Type Dry Gas Std

Standard Value 0.100

Standard Lot Number AG316301-23

Standard Expiration Date 06/12/2015

Tank Pressure 115

Barometric Pressure 762 mmHg

Blow Sample Number 1 Blow Duration 3.95 sec

Blow Volume 2280 cc End-of-Blow Time 12:32

Blow Sample Number 2 Blow Duration 4.06 sec

Blow Volume 2129 cc End-of-Blow Time 12:34

Tamper Evident Stamp 810c3a26

Test Status Code 0

Test Status Success

Ed

Intox EC/IR-II: Accuracy Check

Department of Forensic Science

Serial Number: 010623 Test Number: 939

Test Date: 01/07/2015 Test Time: 12:36 EST

Dry Gas Target: 0.100

Lot Number: AG316301-23 Exp Date: 06/12/2015

Tank Pressure: 115 psi Barometric Pressure: 762 mmHg

System Check: *Passed*

Test	g/210L	Time
BLK	0.000	12:37
CHK	0.101	12:38
BLK	0.000	12:39
CHK	0.101	12:40
BLK	0.000	12:41
CHK	0.101	12:42

Test Status: *Success*

Calibration CRC: 420893D8

Intox EC/IR-II: Accuracy Check

fd

Department of Forensic Science

Serial Number: 010623 Test Number: 940

Test Date: 01/07/2015 Test Time: 12:45 EST

Dry Gas Target: 0.301

Lot Number: AG428003-03 Exp Date: 10/07/2016

Tank Pressure: 144 psi Barometric Pressure: 762 mmHg

System Check: Passed

Test	g/210L	Time
BLK	0.000	12:46
CHK	0.306	12:46
BLK	0.000	12:48
CHK	0.306	12:49
BLK	0.000	12:50
CHK	0.305	12:51

Test Status: Success

Calibration CRC: 420893D8