

Department of Forensic Science
Breath Alcohol Section
Instrument Location History
1/1/1990 To 2/11/2015

Handwritten initials/signature
mm8

Instrument Serial Number: 010462

As of 11-Feb-15

Start Date	End Date	Agency Name
11-Feb-15		DFS Central Lab
28-Aug-14	11-Feb-15	Portsmouth PD
19-Aug-14	28-Aug-14	DFS Central Lab
11-Mar-14	19-Aug-14	Charlotte County SO
23-Sep-13	11-Mar-14	DFS Central Lab
17-Dec-09	23-Sep-13	New Kent County SO
19-Aug-09	17-Dec-09	DFS Central Lab
05-Nov-08	19-Aug-09	Halifax County Sheriff's Office
13-May-08	05-Nov-08	DFS Central Lab

Handwritten initials/signature in the top right corner.

INTOX EC/IR II Quality Assurance Worksheet

Instrument Serial Number: 010462 Worksheet Start Date: 2/11/2015
Location: Portsmouth Police Department
Address: 711 Crawford St., Portsmouth, VA 23704
DFS Technician: Heather Stanton License No.: 18910

Laboratory On-Site

Site Specification: No detrimental environmental conditions exist.

Instrument Barometer (mm HG): 761 Reference Barometer (mm HG): 763
Reference Barometer(RB)Serial #: 009113 RB Calibration Due: 4/28/2015

Measurement Assurance Check


Standard (sea level)	PA Target	minimum	maximum	Sample 1	Sample 2	Sample 3
0.300	0.300	0.291	0.309	0.306	0.305	0.305
Precision		sample min	sample max			
0.001		0.305	0.306			

Standard (sea level)	PA Target	minimum	maximum	Sample 1	Sample 2	Sample 3
0.100	0.100	0.097	0.103	0.100	0.100	0.100
Precision		sample min	sample max			
0		0.100	0.100			


Dry gas standard Lot No. (with tank no.): AG419702-58

- Replaced dry gas standard (+O-ring)
- Installed at Location
- Removed to DFS-Central

Supplies
Mouthpieces
Certificates of Analysis
Operator Worksheet
Other:



Notes:

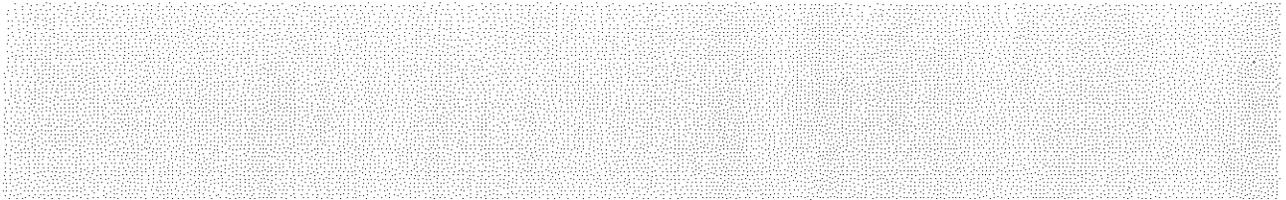

Instrument Serial Number

010462

Certification Date

Calibrated

Certified

Measurement Assurance Check

Instrument Test

Troubleshooting/Maintenance Worksheet Completed

(Successful completion denotes satisfactory condition of the item.)

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.250		0.000	0.000	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.150		0.000	0.000	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.080		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.020		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

All measurements are in g/210L

Estimation of Uncertainty of Measurement and traceability records are located within the Breath Alcohol Section

DFS Technician

Heath M. Stach

Date

2/11/15

Issuing Analyst

Michelle Bell

Date

2/11/15

JPD

lms
mmb



COMMONWEALTH OF VIRGINIA
DEPARTMENT OF FORENSIC SCIENCE

CERTIFICATE OF BLOOD ALCOHOL ANALYSIS
AS DETERMINED BY A CHEMICAL TEST OF THE ACCUSED'S BREATH

NAME OF ACCUSED INSTRUMENT, TEST,	NAME OF COURT DFS
---	-----------------------------

BREATH ANALYSIS

SAMPLE EXAMINED AND TEST CONDUCTED BY STANTON, HEATHER, M		AGENCY DFS Central Lab
DFS LICENSE NUMBER 18910	LICENSE EXPIRES 10/01/2016	DATE TEST CONDUCTED 02/11/2015
TEST EQUIPMENT NUMBER 010462		

RESULTS: TIME SAMPLE TAKEN 10:09 EST

SAMPLE'S ALCOHOL CONTENT 0.00 GRAMS PER 210 LITERS OF BREATH

ATTEST:

I CERTIFY THAT THE ABOVE IS AN ACCURATE RECORD OF THE TEST CONDUCTED; THAT THE TEST WAS CONDUCTED WITH THE TYPE OF EQUIPMENT AND IN ACCORDANCE WITH THE METHODS APPROVED BY THE DEPARTMENT OF FORENSIC SCIENCE; THAT THE TEST WAS CONDUCTED IN ACCORDANCE WITH THE DEPARTMENT'S SPECIFICATIONS; THAT PRIOR TO ADMINISTRATION OF THE TEST THE ACCUSED WAS ADVISED OF HIS RIGHT TO OBSERVE THE PROCESS AND SEE THE BLOOD ALCOHOL READING ON THE EQUIPMENT USED TO PERFORM THE BREATH TEST, AND THAT I POSSESS A VALID LICENSE TO CONDUCT SUCH TEST, GIVEN UNDER MY HAND THIS _____ DAY OF _____, 20 _____.

BREATH TEST OPERATOR

I HAVE RECEIVED A COPY OF THIS CERTIFICATE OF ANALYSIS _____ SUBJECT'S SIGNATURE

SUBJECT REFUSED TO SIGN FOR COPY OF CERTIFICATE OF ANALYSIS _____ OPERATOR'S SIGNATURE



IntoxNet MIS Report

Report Generated 11 Feb 2015 at 10:36

nmb
HMS

Test Results

Instrument Serial Number 010462

Test # 000724 Subject Test

Test Location 1 Department of
Test Date 11 Feb 2015

Test Location 2 Forensic Science
Test Time 10:03
Remote/Local Local

Test Location 3
System Check Passed

Operator's Last Name STANTON
Agency DFS Central Lab

Operator's First Name HEATHER

Operator's Middle Initial *N*

Card Serial Number 118910

License Number 18910

Effective Date 10/01/2014

Expiration Date 10/01/2016

Subject's Last Name INSTRUMENT

Subject's First Name TEST

Subject's Middle Initial

Subject's Date of Birth 00/00/0000

Subject's Sex Male

Driver's License Number

Driver's License Expiration 00/00/0000

Driver's License State

Court Name DFS

End Date 11 Feb 2015 End Time 10:10

Result Time 10:09

Result Date 11 Feb 2015 Result 0.00

Data Type DIAG

Sample Value Pass

Sample Time 10:03

Data Type BLK

Sample Value 0.000

Sample Time 10:04

Data Type CHK

Sample Value 0.100

Sample Time 10:04

Data Type BLK

Sample Value 0.000

Sample Time 10:06

Data Type SUBJ

Sample Value 0.000

Sample Time 10:07

Data Type BLK

Sample Value 0.000

Sample Time 10:08

Data Type SUBJ

Sample Value 0.000

Sample Time 10:09

Data Type BLK

Sample Value 0.000

Sample Time 10:10

Standard Type Dry Gas Std

Standard Value 0.100

Standard Lot Number AG419702-58

Standard Expiration Date 07/16/2016

Tank Pressure 860

Barometric Pressure 761 mmHg

Blow Sample Number 1 Blow Duration 3.14 sec

Blow Volume 1798 cc End-of-Blow Time 10:07

Blow Sample Number 2 Blow Duration 3.28 sec

Blow Volume 1800 cc End-of-Blow Time 10:09

Tamper Evident Stamp 0287ea81

Test Status Code 0

Test Status Success

~~KMS~~
mmB

Intox EC/IR-II: Accuracy Check

Department of Forensic Science

Serial Number: 010462 Test Number: 725

Test Date: 02/11/2015 Test Time: 10:13 EST

Dry Gas Target: 0.100

Lot Number: AG419702-58 Exp Date: 07/16/2016

Tank Pressure: 855 psi Barometric Pressure: 761 mmHg

System Check: *Passed*

Test	g/210L	Time
BLK	0.000	10:13
CHK	0.100	10:14
BLK	0.000	10:16
CHK	0.100	10:17
BLK	0.000	10:18
CHK	0.100	10:19

Test Status: *Success*

Calibration CRC: 6550E25C

KMS
mmB

Intox EC/IR-II: Accuracy Check

Department of Forensic Science

Serial Number: 010462 Test Number: 726

Test Date: 02/11/2015 Test Time: 10:21 EST

Dry Gas Target: 0.300

Lot Number: AG428003-07 Exp Date: 10/07/2016

Tank Pressure: 262 psi Barometric Pressure: 761 mmHg

System Check: *Passed*

Test	g/210L	Time
BLK	0.000	10:22
CHK	0.306	10:23
BLK	0.000	10:25
CHK	0.305	10:25
BLK	0.000	10:27
CHK	0.305	10:28

Test Status: *Success*

Calibration CRC: 6550E25C