

Handwritten initials/signature

INTOX EC/IR II Quality Assurance Worksheet

Instrument Serial Number **010485** Worksheet Start Date **4/6/2015**

Location **Arlington Police Department**

Address **1425 N. Courthouse Rd., Arlington, VA 22201**

DFS Technician **Heather Stanton** License No. **18910**

Laboratory On-Site

Site Specification: No detrimental environmental conditions exist.

Instrument Barometer (mm HG) **764** Reference Barometer (mm HG) **762**

Reference Barometer(RB)Serial # **009113** RB Calibration Due **4/28/2015**

Measurement Assurance Check

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.300		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.100		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	


Dry gas standard Lot No. (with tank no.) **AG332301-14**

- Replaced dry gas standard (+O-ring)
- Installed at Location
- Removed to DFS-Central

Supplies
Mouthpieces
Certificates of Analysis
Operator Worksheet
Other:



Notes:

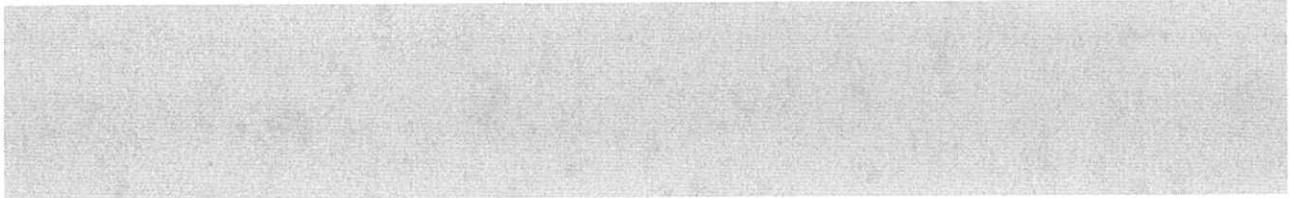

Instrument Serial Number

010485

Certification Date

Calibrated

Certified

Measurement Assurance Check

Instrument Test

Troubleshooting/Maintenance Worksheet Completed

(Successful completion denotes satisfactory condition of the item.)

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.250		0.000	0.000	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.150		0.000	0.000	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.080		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.020		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

All measurements are in g/210L

Estimation of Uncertainty of Measurement and traceability records are located within the Breath Alcohol Section

DFS Technician

Heath M. Stach

Date

4/6/15

Issuing Analyst

gld
TLN

Date

4/7/15

AMS
nd



COMMONWEALTH OF VIRGINIA
DEPARTMENT OF FORENSIC SCIENCE

CERTIFICATE OF BLOOD ALCOHOL ANALYSIS
AS DETERMINED BY A CHEMICAL TEST OF THE ACCUSED'S BREATH

NAME OF ACCUSED INSTRUMENT, TEST,	NAME OF COURT DFS
--	--------------------------

BREATH ANALYSIS

SAMPLE EXAMINED AND TEST CONDUCTED BY STANTON, HEATHER, M		AGENCY DFS Central Lab
DFS LICENSE NUMBER 18910	LICENSE EXPIRES 10/01/2016	DATE TEST CONDUCTED 04/06/2015
TEST EQUIPMENT NUMBER 010485		

RESULTS: TIME SAMPLE TAKEN 12:06 EDT

SAMPLE'S ALCOHOL CONTENT 0.00 GRAMS PER 210 LITERS OF BREATH

ATTEST:

I CERTIFY THAT THE ABOVE IS AN ACCURATE RECORD OF THE TEST CONDUCTED; THAT THE TEST WAS CONDUCTED WITH THE TYPE OF EQUIPMENT AND IN ACCORDANCE WITH THE METHODS APPROVED BY THE DEPARTMENT OF FORENSIC SCIENCE; THAT THE TEST WAS CONDUCTED IN ACCORDANCE WITH THE DEPARTMENT'S SPECIFICATIONS; THAT PRIOR TO ADMINISTRATION OF THE TEST THE ACCUSED WAS ADVISED OF HIS RIGHT TO OBSERVE THE PROCESS AND SEE THE BLOOD ALCOHOL READING ON THE EQUIPMENT USED TO PERFORM THE BREATH TEST, AND THAT I POSSESS A VALID LICENSE TO CONDUCT SUCH TEST, GIVEN UNDER MY HAND THIS _____ DAY OF _____, 20 _____.

BREATH TEST OPERATOR

I HAVE RECEIVED A COPY OF THIS CERTIFICATE OF ANALYSIS _____ SUBJECT'S SIGNATURE

SUBJECT REFUSED TO SIGN FOR COPY OF CERTIFICATE OF ANALYSIS _____ OPERATOR'S SIGNATURE



IntoxNet MIS Report

Report Generated 06 Apr 2015 at 15:41

Handwritten initials: HNS and Jd

Test Results

Instrument Serial Number 010485

Test # 002158	Subject Test	Test Location 2 Forensic Science	Test Location 3
Test Location 1 Department of		Test Time 12:00	System Check Passed
Test Date 06 Apr 2015		Remote/Local Local	
Operator's Last Name STANTON		Operator's First Name HEATHER	Operator's Middle Initial M
Agency DFS Central Lab		License Number 18910	
Card Serial Number 118910		Effective Date 10/01/2014	Expiration Date 10/01/2016
Subject's Last Name INSTRUMENT		Subject's First Name TEST	
Subject's Middle Initial		Subject's Date of Birth 00/00/0000	Subject's Sex Male
Driver's License Number		Driver's License Expiration 00/00/0000	
Driver's License State		Court Name DFS	
End Date 06 Apr 2015	End Time 12:07	Result Time 12:06	Result Date 06 Apr 2015
Data Type DIAG		Sample Value Pass	Sample Time 12:00
Data Type BLK		Sample Value 0.000	Sample Time 12:01
Data Type CHK		Sample Value 0.100	Sample Time 12:02
Data Type BLK		Sample Value 0.000	Sample Time 12:03
Data Type SUBJ		Sample Value 0.000	Sample Time 12:04
Data Type BLK		Sample Value 0.000	Sample Time 12:05
Data Type SUBJ		Sample Value 0.000	Sample Time 12:06
Data Type BLK		Sample Value 0.000	Sample Time 12:07
Standard Type Dry Gas Std		Standard Value 0.101	
Standard Lot Number AG332301-14		Standard Expiration Date 11/19/2015	
Tank Pressure 473		Barometric Pressure 764 mmHg	
Blow Sample Number 1	Blow Duration 3.19 sec	Blow Volume 1746 cc	End-of-Blow Time 12:04
Blow Sample Number 2	Blow Duration 3.31 sec	Blow Volume 1728 cc	End-of-Blow Time 12:06
Tamper Evident Stamp c41014c0		Test Status Code 0	
Test Status Success			